

Sample Name :Cardiotoxin Analog (CTX) IV (6-12)  
 Cat. No. : RP17303  
 Lot. No. :PE8381704

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

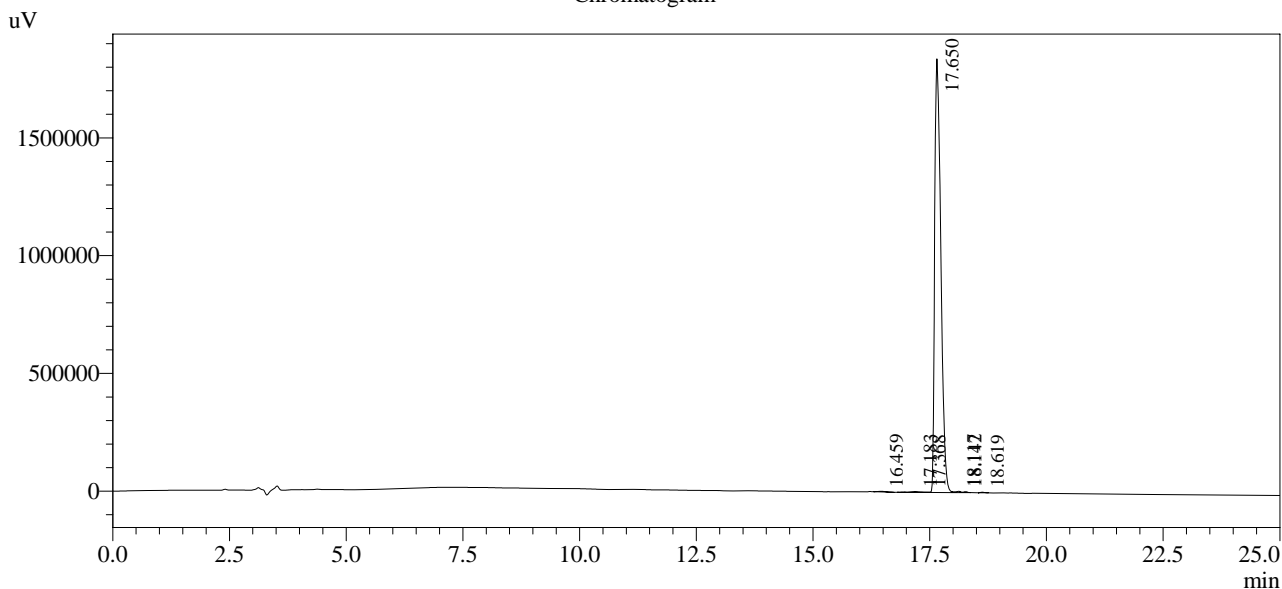

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	16.459	26458	2370	0.155
2	17.183	53033	3446	0.310
3	17.368	12252	1611	0.072
4	17.650	16934564	1840945	98.981
5	18.117	39490	5302	0.231
6	18.142	30808	4833	0.180
7	18.619	12268	2446	0.072
Total		17108873	1860954	100.000