

Sample Name :DYKDDDDK Peptide
 Cat. No. : RP10586
 Lot. No. : E3393319H
 Time Processed :14:48:07
 Month-Day-Year Processed :08/16/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	0	
5.00	Pumps	Pump B Conc.	0	
20.00	Pumps	Pump B Conc.	30	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	0	
40.00	Pumps	Pump B Conc.	0	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment :SS-CM-0310

Chromatogram

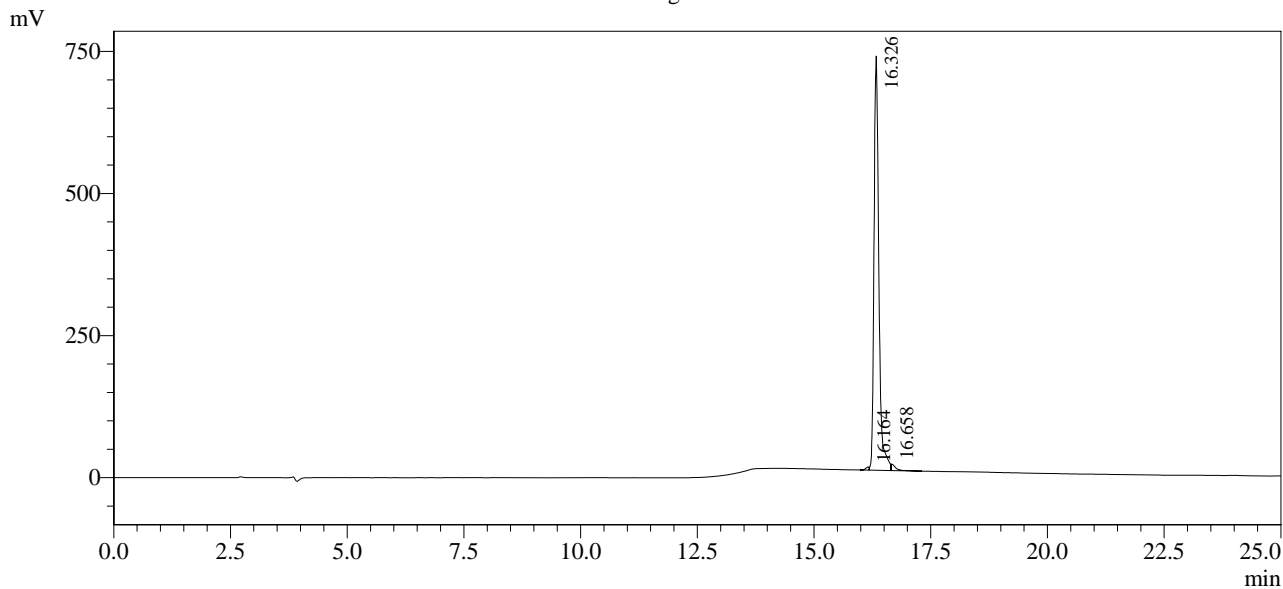

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	16.164	28424	5540	0.530
2	16.326	5260032	728980	98.064
3	16.658	75442	11429	1.406
Total		5363898	745949	100.000