

Sample Name : Calcitonin Gene Related Peptide (CGRP) (8-37), human
 Cat No.: RP11089
 Lot No.: E7124220L
 Time Processed : 15:02:05
 Month-Day-Year Processed : 12/24/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010509

<Chromatogram>

mV

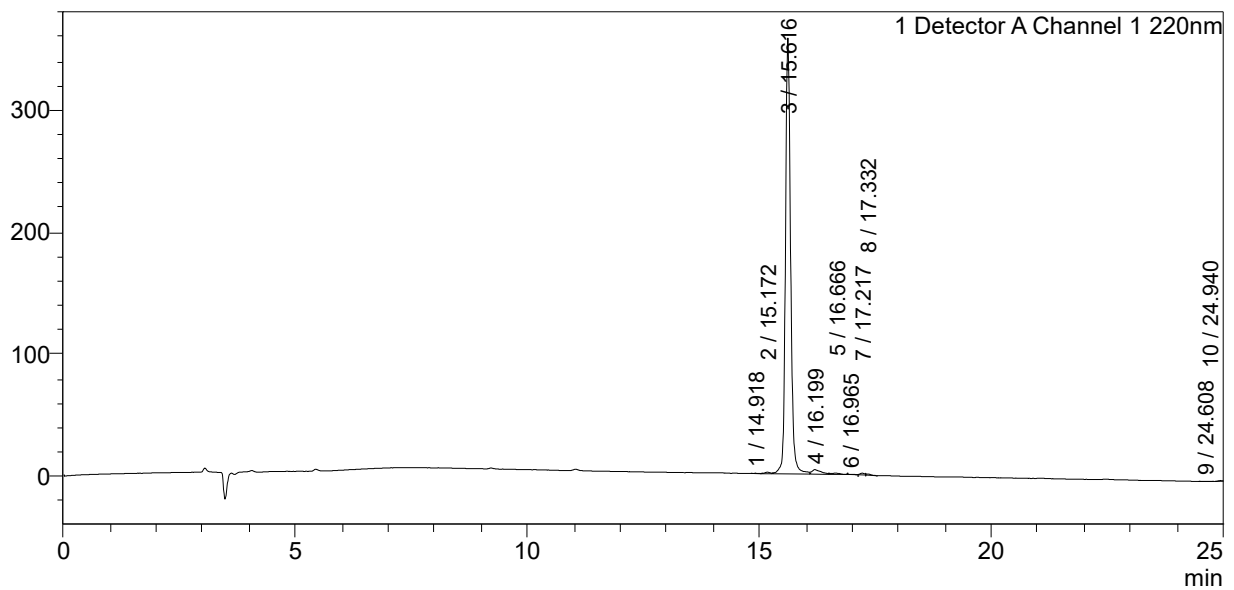

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.918	1136	224	0.040
2	15.172	9281	1255	0.323
3	15.616	2776463	357347	96.572
4	16.199	52071	3747	1.811
5	16.666	13229	965	0.460
6	16.965	1857	217	0.065
7	17.217	10419	1459	0.362
8	17.332	5974	956	0.208
9	24.608	1459	163	0.051
10	24.940	3118	532	0.108
Total		2875008	366866	100.000