

Sample Name :Angiotensin II, human
Cat. No. : RP11257 Lot. No. : PE5401808

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

<Chromatogram>

mV

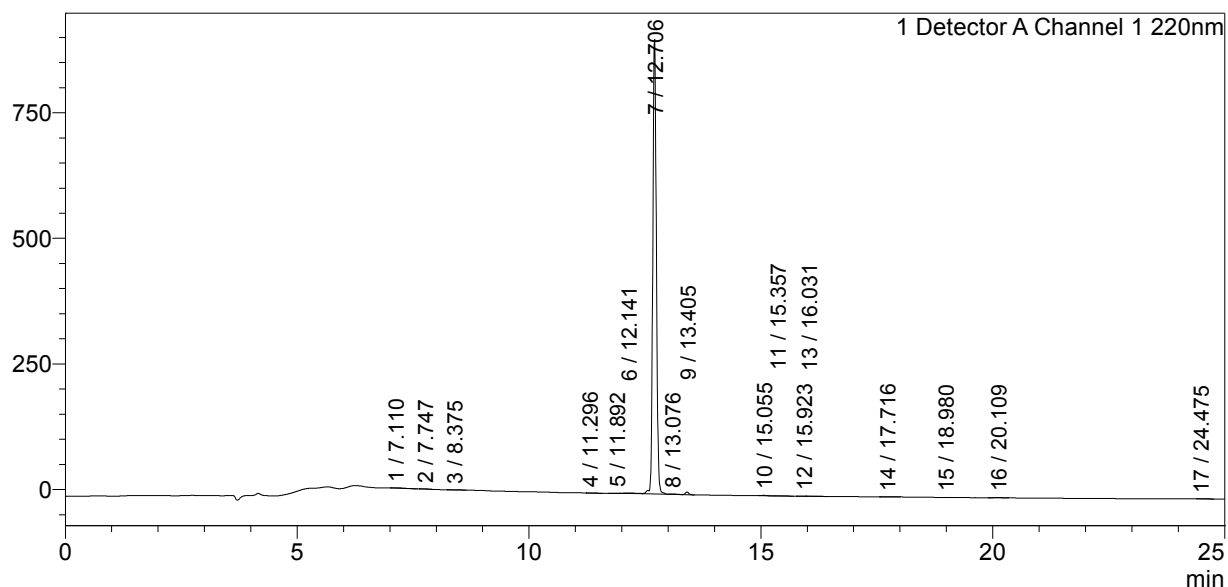

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	7.110	11337	633	0.232
2	7.747	5819	575	0.119
3	8.375	3278	240	0.067
4	11.296	2153	255	0.044
5	11.892	2580	306	0.053
6	12.141	15532	953	0.317
7	12.706	4789691	905271	97.888
8	13.076	7409	831	0.151
9	13.405	26276	4952	0.537
10	15.055	4745	742	0.097
11	15.357	1773	119	0.036
12	15.923	1939	242	0.040
13	16.031	5374	361	0.110
14	17.716	1805	158	0.037
15	18.980	2312	173	0.047
16	20.109	9173	844	0.187
17	24.475	1819	126	0.037

Peak#	Ret. Time	Area	Height	Area%
Total		4893016	916780	100.000