

Sample Name :Hexa-His  
 Cat No.: RP11737  
 Lot No.:E5874820E  
 Time Processed :9:39:44  
 Month-Day-Year Processed :05/24/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	0
25.00	Pumps	Pump A B.Conc	50
25.01	Pumps	Pump A B.Conc	95
32.00	Pumps	Pump A B.Conc	95
32.01	Pumps	Pump A B.Conc	0
40.00	Pumps	Pump A B.Conc	0
45.00	Controller	Stop	

<<Column Performance>>

<Detector A>  
 Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ19010324

<Chromatogram>

mV

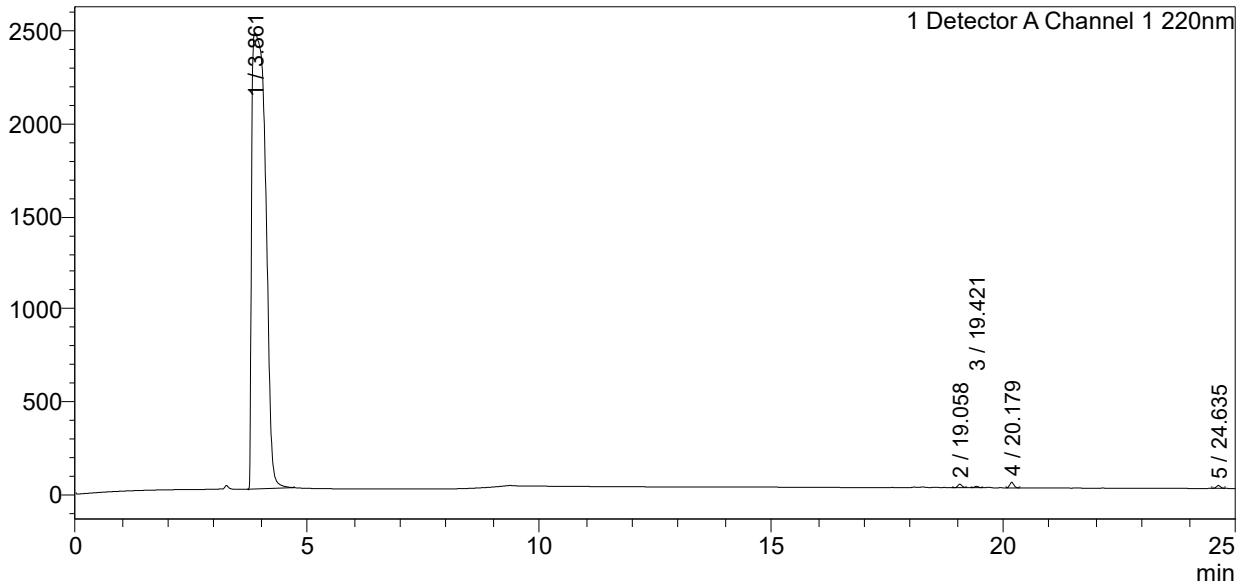

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	3.861	50807862	2464119	99.163
2	19.058	108963	18426	0.213
3	19.421	44093	7823	0.086
4	20.179	183813	30434	0.359
5	24.635	92234	14978	0.180
Total		51236965	2535781	100.000