

Sample Name :Transportan
 Cat No. :RP20512
 Lot No. :E4277319G
 Time Processed :5:53:22
 Month-Day-Year Processed :07/25/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

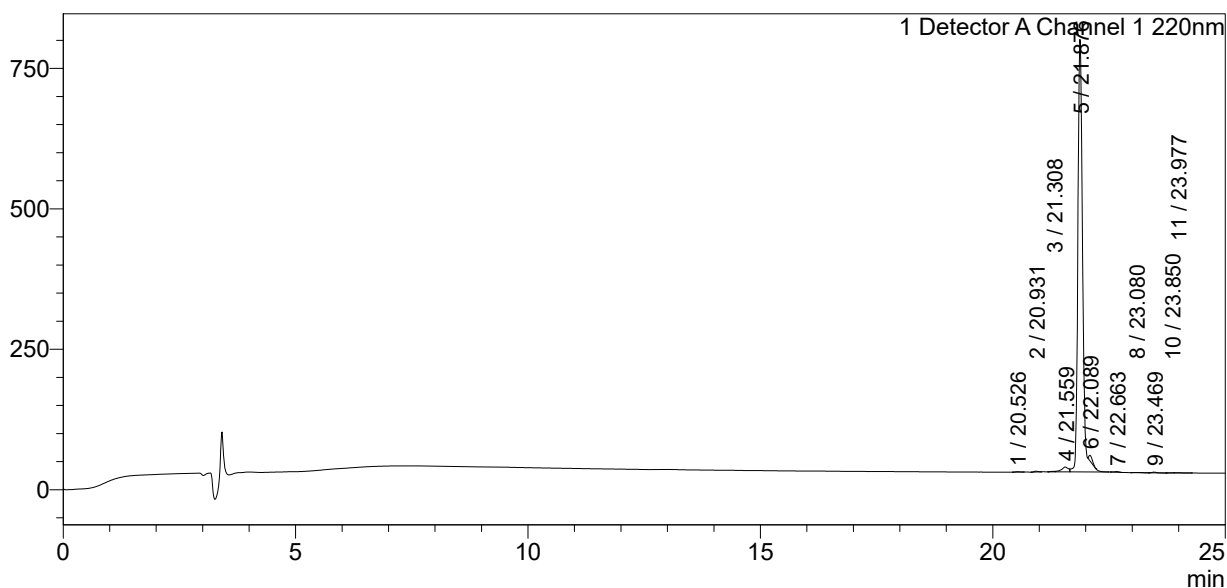

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	20.526	4181	660	0.074
2	20.931	8581	1508	0.152
3	21.308	5838	997	0.104
4	21.559	89428	8630	1.588
5	21.876	5444807	770025	96.701
6	22.089	50092	9752	0.890
7	22.663	8360	1173	0.148
8	23.080	4397	430	0.078
9	23.469	8158	1367	0.145
10	23.850	2029	340	0.036
11	23.977	4678	568	0.083
Total		5630549	795450	100.000