

Sample Name : β -Amyloid (13-27)
 Cat. No. : RP20170
 Lot. No. : E4830019I
 Time Processed : 14:21:21
 Month-Day-Year Processed : 09/21/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment : SS-CM-0310

Chromatogram

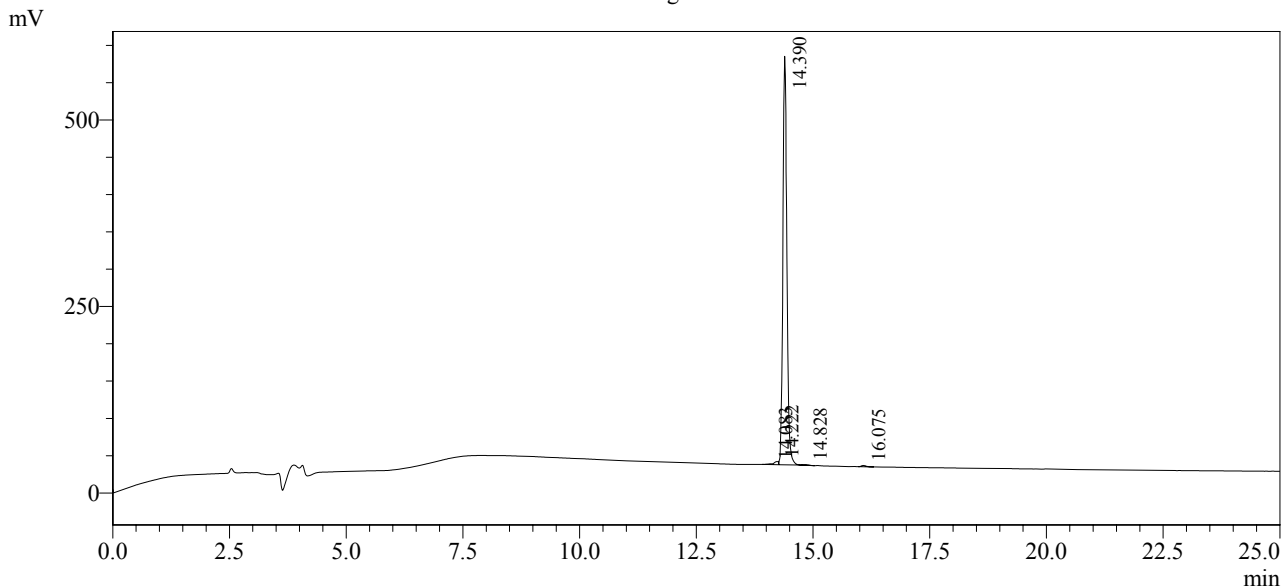

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.083	6646	975	0.200
2	14.222	26310	4110	0.793
3	14.390	3265061	547678	98.456
4	14.828	6195	818	0.187
5	16.075	12039	1724	0.363
Total		3316251	555305	100.000