

Sample Name :Gastrin-1, human
 Cat. No. : RP12740
 Lot. No. : E8750020K

Time Processed : 10:19:23 AM
 Month-Day-Year Processed : 12/03/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
32.00	Pumps	B.Conc	95
32.01	Pumps	B.Conc	5
40.00	Pumps	B.Conc	5
45.00	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK11010017

mV

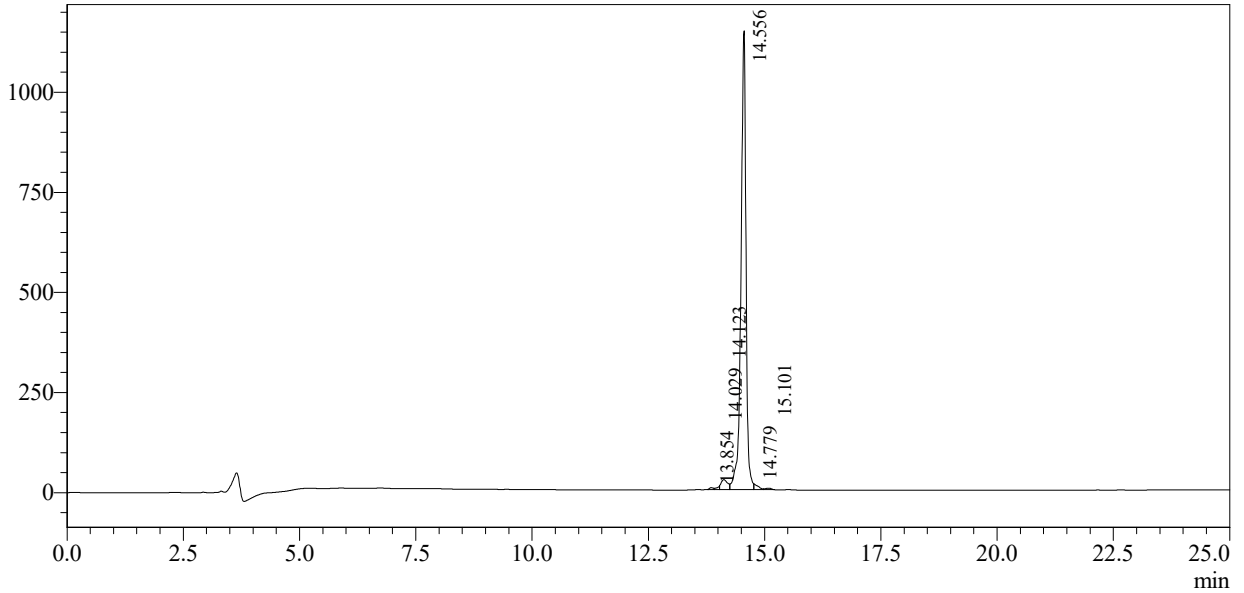

1 Detector A Channel 1 / 220nm

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.854	26302	4423	0.292
2	14.029	34249	7744	0.380
3	14.123	241746	24540	2.685
4	14.556	8587589	1145431	95.392
5	14.779	84332	13758	0.937
6	15.101	28203	3113	0.313
Total		9002421	1199009	100.000