

Sample Name : InsB 9-23
 Cat. No. : RP20391
 Lot. No. : E6897620H
 Time Processed : 19:10:37
 Month-Day-Year Processed : 08/07/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0309

Chromatogram

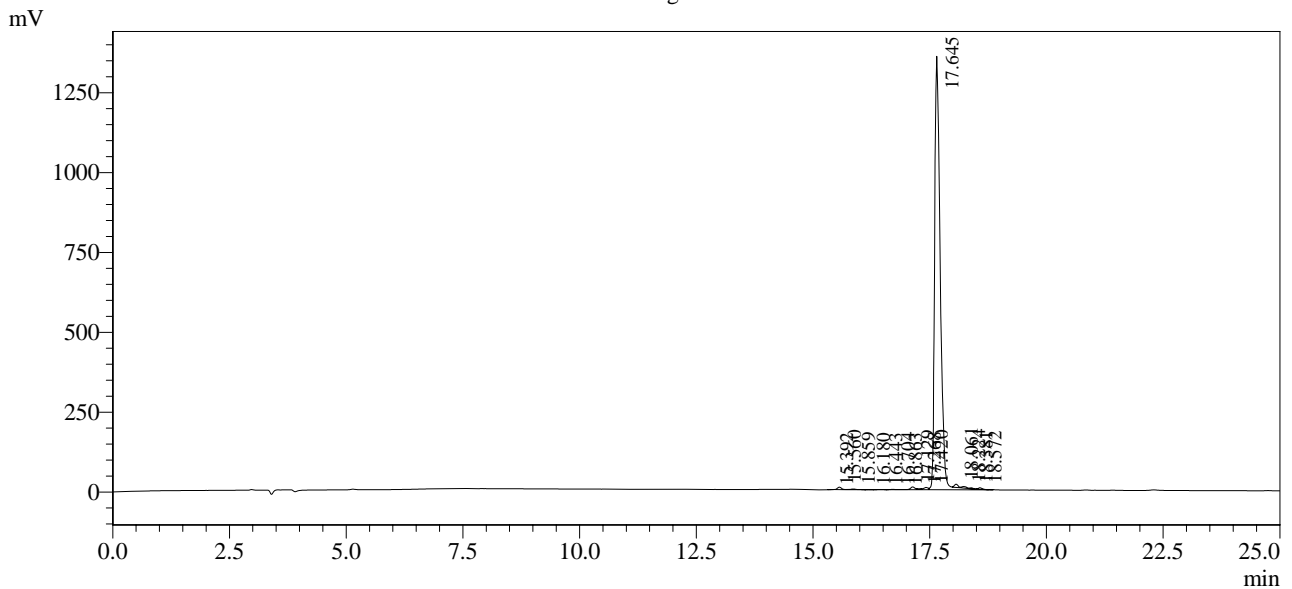

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	15.392	894	244	0.008
2	15.560	47612	7698	0.407
3	15.859	16991	2012	0.145
4	16.180	1170	147	0.010
5	16.443	4556	489	0.039
6	16.704	8222	993	0.070
7	16.863	3254	492	0.028
8	17.129	60448	8621	0.517
9	17.268	17486	3292	0.150
10	17.420	52537	7143	0.450
11	17.645	11336889	1357006	97.021
12	18.061	56307	10201	0.482
13	18.224	35292	4706	0.302
14	18.381	14082	2744	0.121
15	18.572	29259	4920	0.250
Total		11684999	1410707	100.000