


# Mass Spectrum

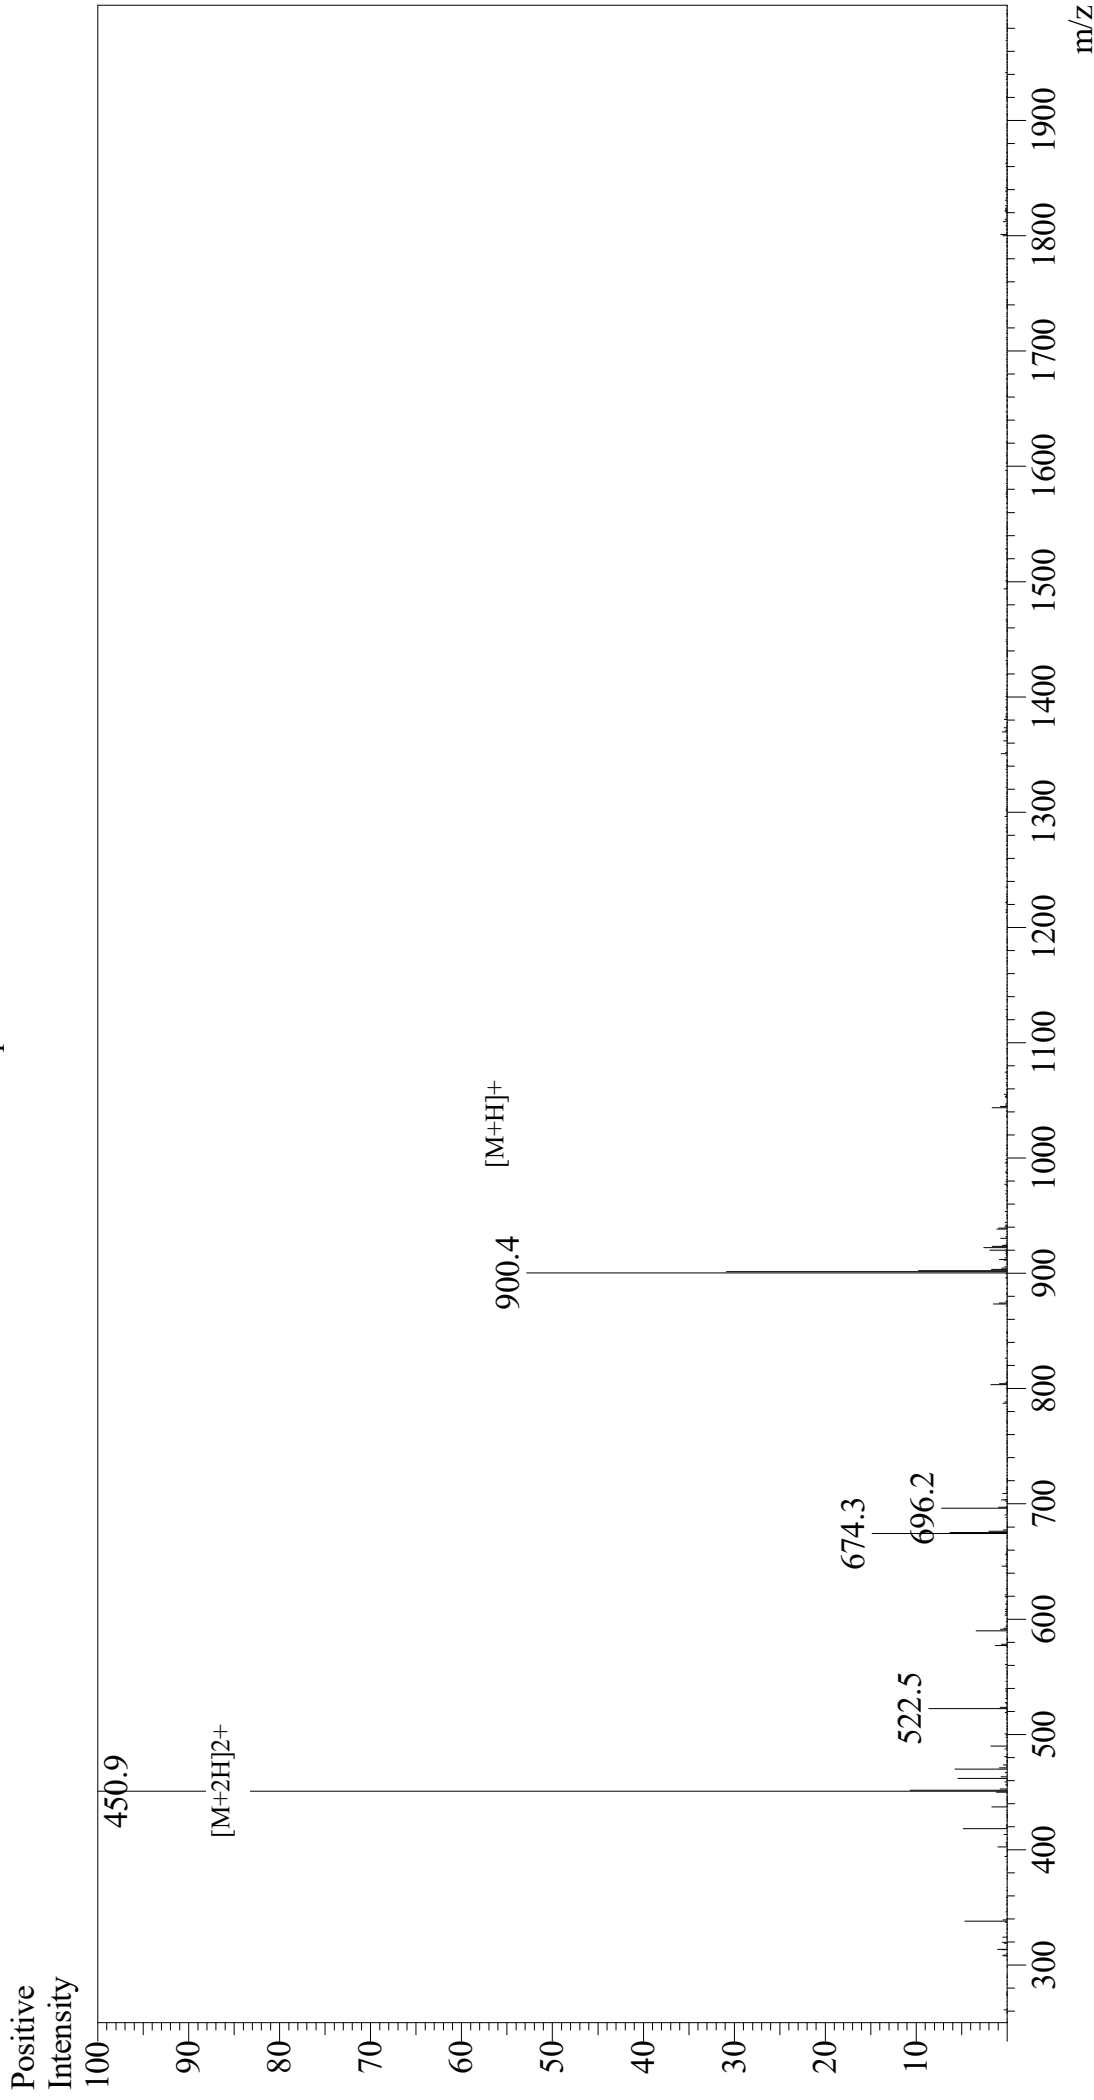

Sample Information  
Month-Day Processed : 01/06/21  
Time Processed : 8:47:45 PM  
Injection Volume : 0.3  
Sample Name : Cardiotoxin Analog (CTX) IV (6-12)  
Cat No. : RP17303  
Lot No. : E4940120L  
Theoretical MW : 899.14  
Observed MW : 899.8

Interface : ESI  
Nebulizing Gas Flow : 1.5L/min  
CDL Temp : 250  
Block Temp : 200  
Equipment : GK11010007  
Interface Bias : +3.5 kV  
Drying Gas Flow : 5 L/min  
T.Flow : 0.2 ml/min  
B.conc : 50%H2O/50%MeOH