

Sample Name :Influenza NP (147-155)  
 Cat No: RP20260  
 Lot No :E2831021E  
 Time Processed :2:17:51 PM  
 Month-Day-Year Processed :05/09/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
31.00	Pumps	B.Conc	95
31.01	Pumps	B.Conc	5
40.00	Pumps	B.Conc	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010140

<Chromatogram>

mV

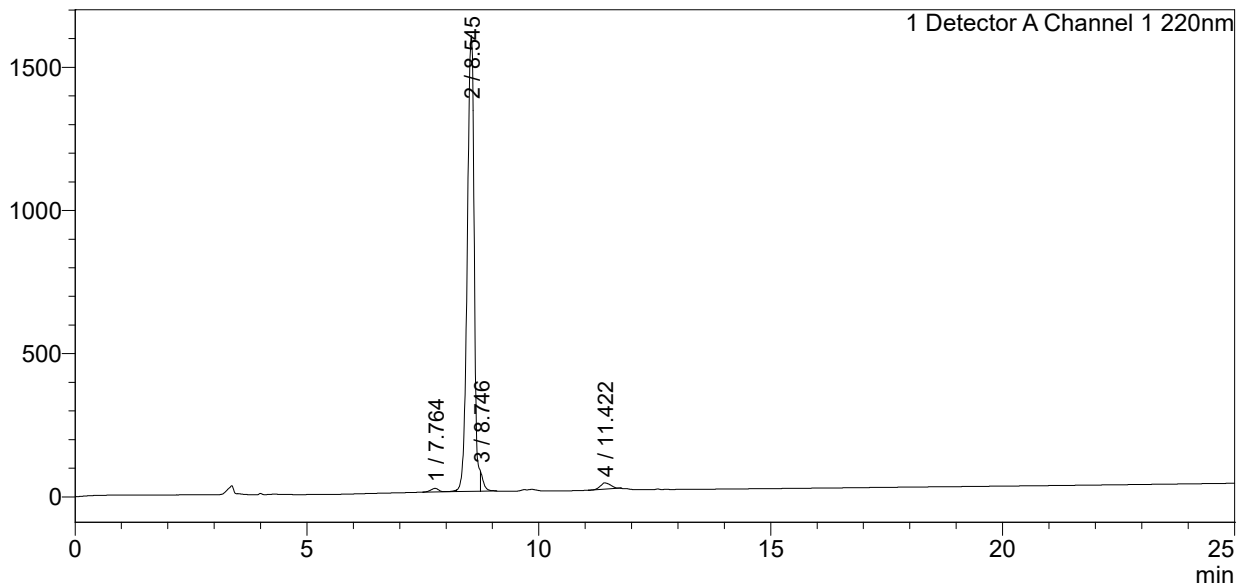

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	7.764	176305	12343	1.017
2	8.545	16534901	1591780	95.375
3	8.746	290407	69799	1.675
4	11.422	335160	22247	1.933
Total		17336773	1696168	100.000