


Mass Spectrum

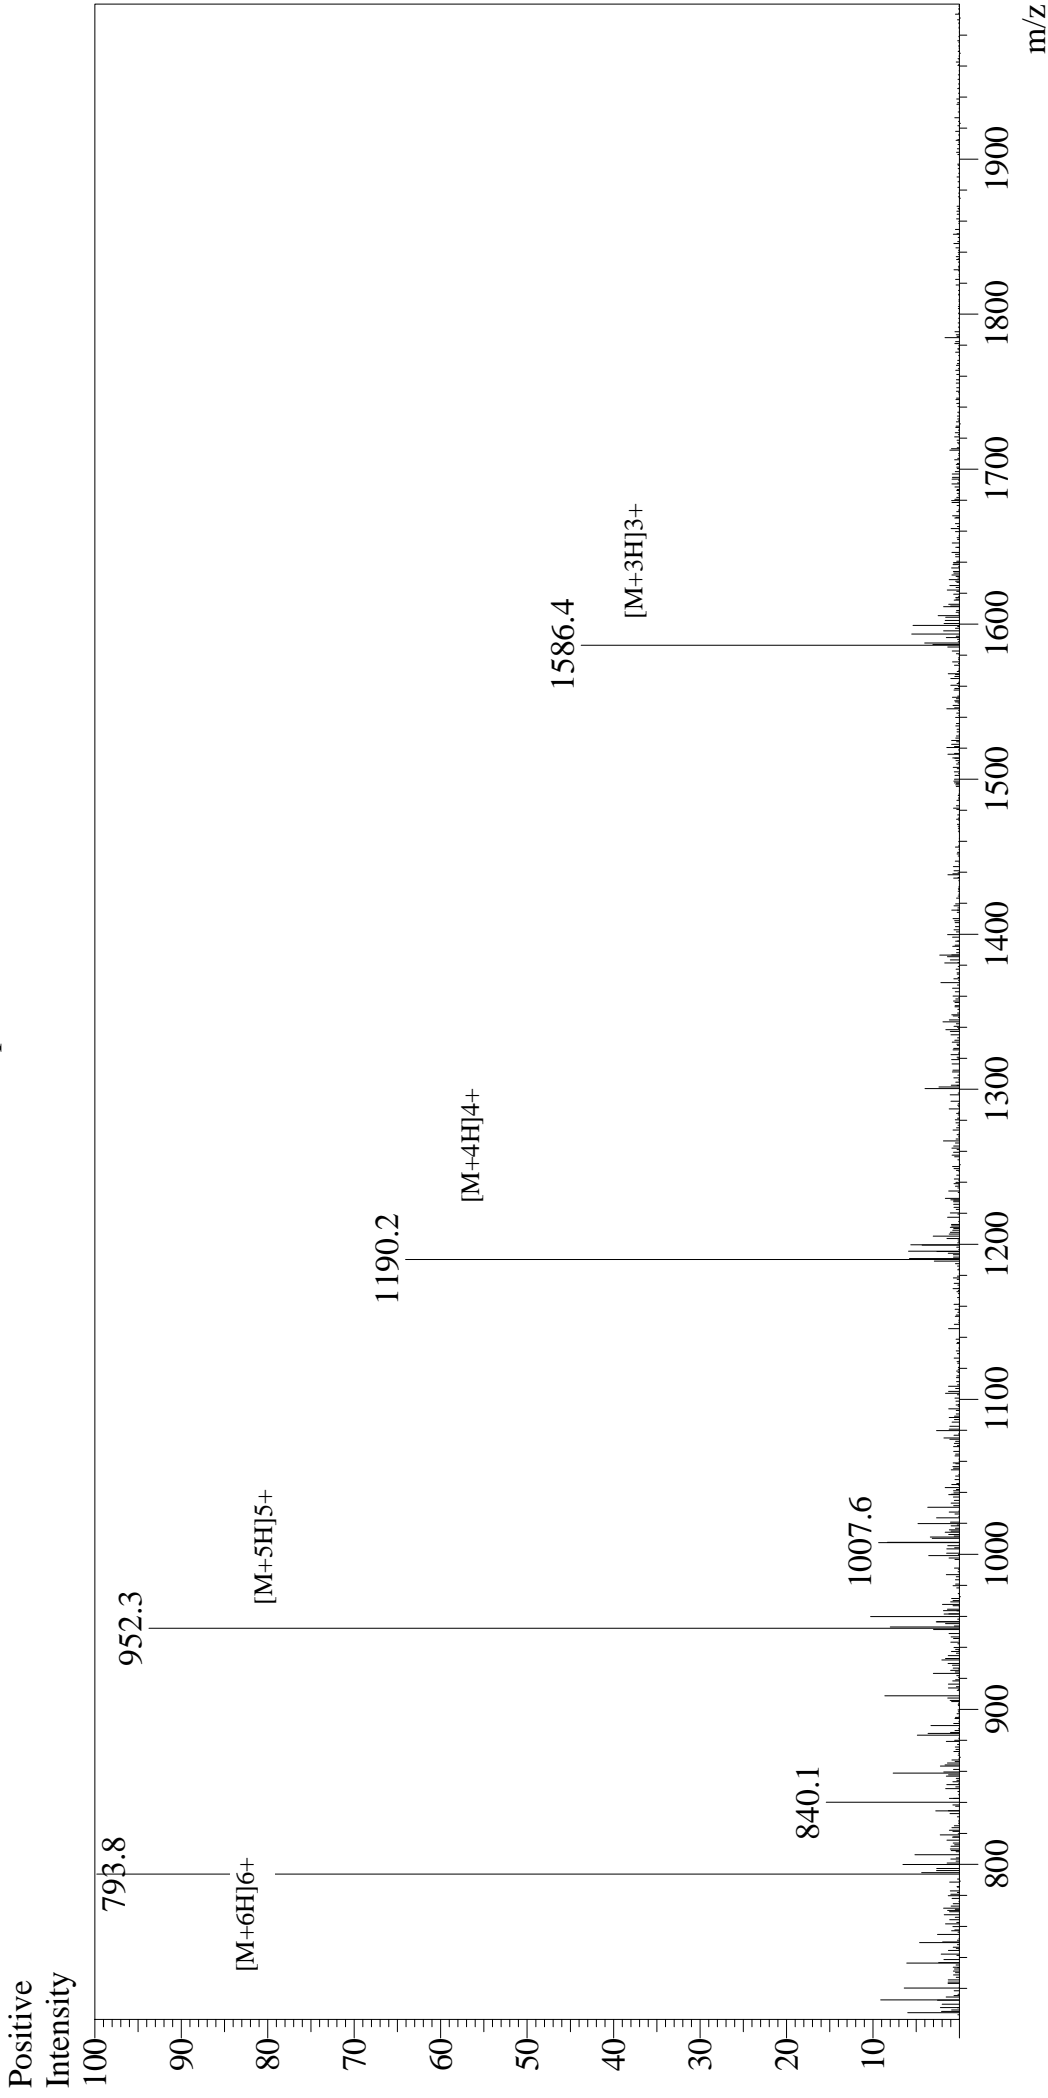

Sample Information

User : Gary
 Month-Day Processed : 07/03/20
 Time Processed : 19:22:36
 Injection Volume : 0.3
 Sample Name : Corticotropin Releasing Factor, human, rat
 Cat No. : RP10982
 Lot No. : E3446820G
 Theoretical MW : 4757.45
 Observed MW : 4756.8

Interface : ESI
 Nebulizing Gas Flow : 1.5L/min
 CDL Temp : 250
 Block Temp : 200

Equipment : GK11010007
 Interface Bias : +4.5kV
 Drying Gas Flow : 5 L/min
 T.Flow : 0.2ml/min
 B.conc : 50%H2O/50%MeOH