

Sample Name :Angiotensin II, human  
 Cat. No. : RP11257  
 Lot. No. : PE2441810  
 Time Processed : 19:18:35  
 Month-Day-Year Processed : 10/11/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	15	
25.00	Pumps	Pump B Conc.	75	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

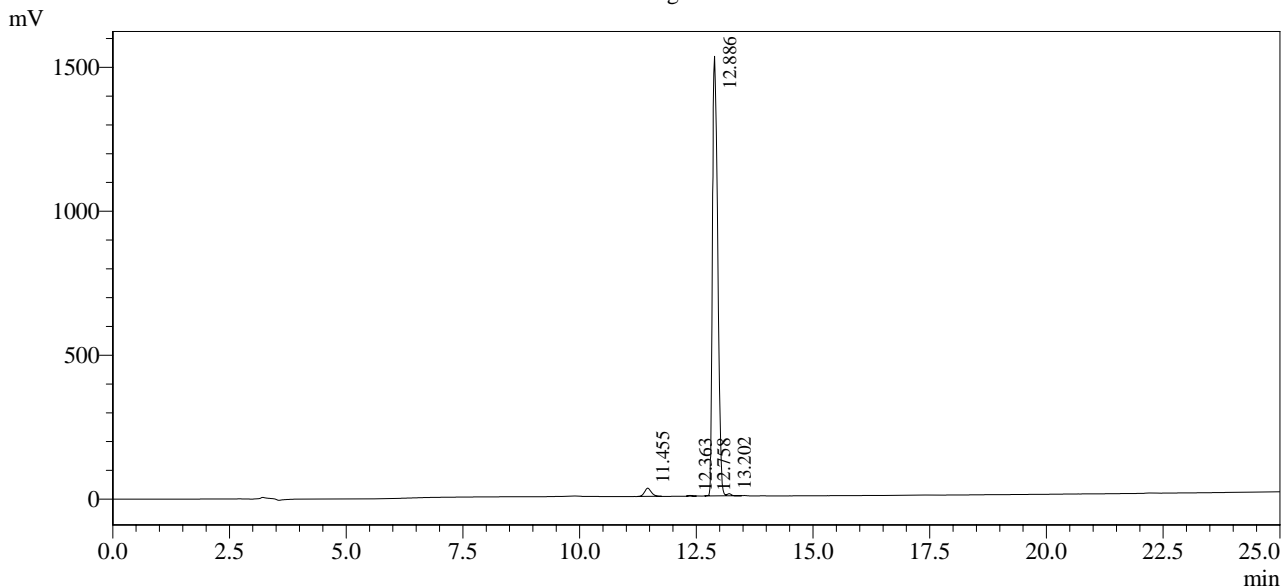

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.455	287045	28664	2.319
2	12.363	12012	2492	0.097
3	12.758	5715	1883	0.046
4	12.886	12028300	1527116	97.162
5	13.202	46622	7441	0.377
Total		12379693	1567597	100.000