

Sample Name :Gly-Arg-Gly-Asp-Ser
 Cat No :RP10848
 Lot No :E7326821C
 Time Processed :10:34:26 PM
 Month-Day-Year Processed :03/21/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	0
5.00	Pumps	Pump A B.Conc	0
20.00	Pumps	Pump A B.Conc	30
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	0
35.00	Pumps	Pump A B.Conc	0
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK11010011

<Chromatogram>

mV

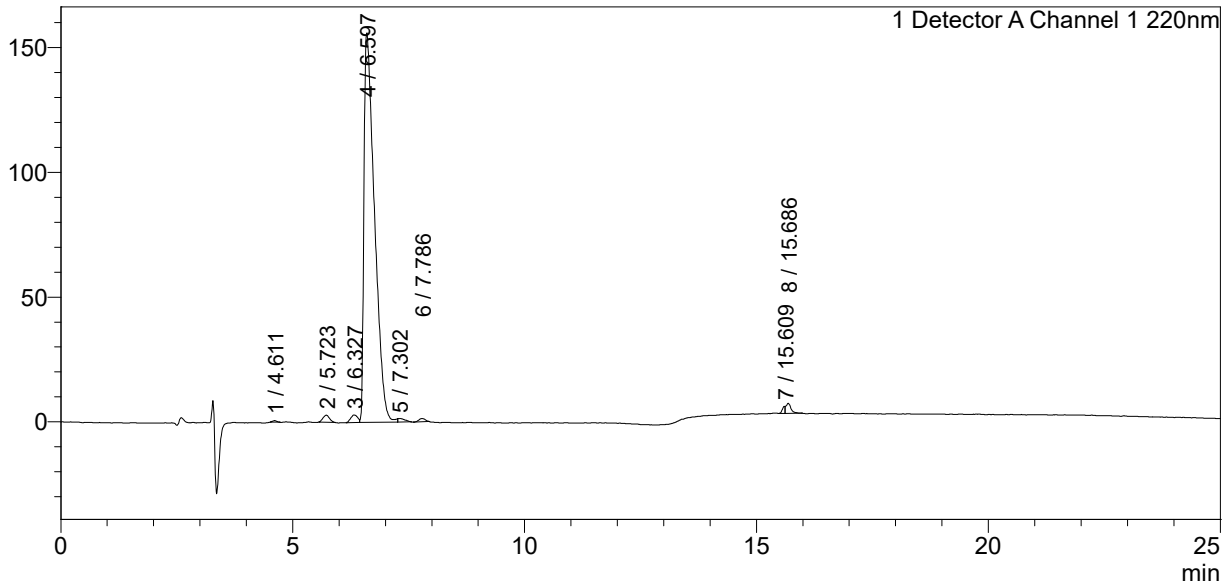

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	4.611	3661	595	0.141
2	5.723	26827	2796	1.037
3	6.327	31368	3039	1.212
4	6.597	2458825	156219	95.007
5	7.302	13988	1401	0.541
6	7.786	12511	1296	0.483
7	15.609	11470	2809	0.443
8	15.686	29400	3983	1.136
Total		2588051	172139	100.000