

Sample Name :Dynorphin A(1-13), porcine
 Cat No.: RP20492
 Lot No.:E4977019J
 Time Processed :14:48:48
 Month-Day-Year Processed :10/03/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	5
40.00	Pumps	Solvent B Conc.	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

mV

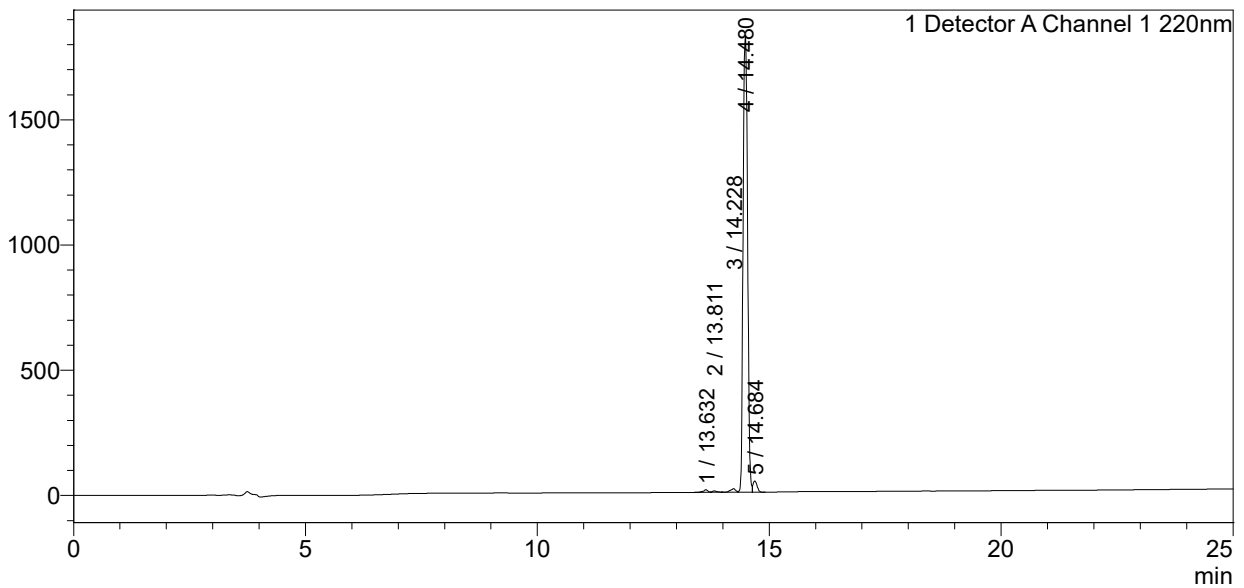

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.632	73899	10680	0.577
2	13.811	41995	6200	0.328
3	14.228	123178	14463	0.962
4	14.480	12291364	1822583	95.962
5	14.684	278176	45289	2.172
Total		12808612	1899214	100.000