

Sample Name :Axltide
 Cat. No. : RP20363
 Lot. No. :E6544020B
 Time Processed :11:01:11
 Month-Day-Year Processed :02/21/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment :SS-CM-0310

Chromatogram

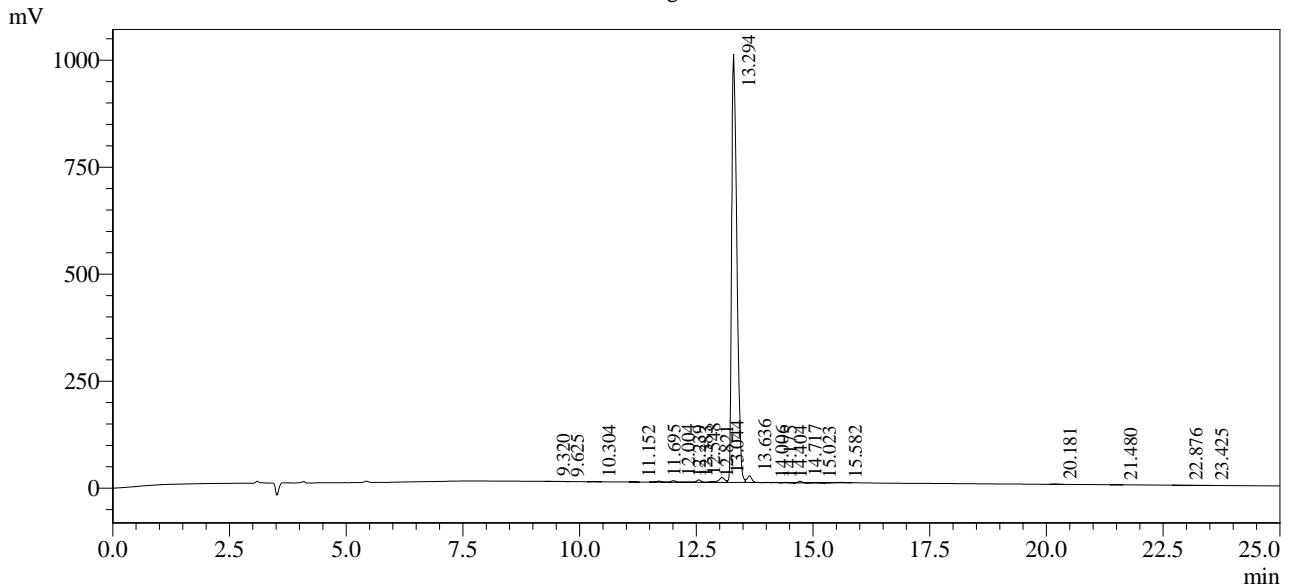

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.320	1672	294	0.020
2	9.625	1469	310	0.018
3	10.304	2904	436	0.035
4	11.152	1244	223	0.015
5	11.695	19977	2561	0.243
6	12.004	24541	3821	0.299
7	12.239	3185	446	0.039
8	12.383	2582	388	0.031
9	12.548	37501	5840	0.456
10	12.821	13501	1693	0.164
11	13.044	102492	11490	1.247
12	13.294	7830317	1000525	95.270
13	13.636	109089	15429	1.327
14	14.006	2014	370	0.025
15	14.175	3036	542	0.037
16	14.404	5053	741	0.061
17	14.717	22506	3695	0.274
18	15.023	3502	467	0.043
19	15.582	16626	972	0.202
20	20.181	5424	857	0.066
21	21.480	2444	361	0.030
22	22.876	6359	351	0.077
23	23.425	1653	281	0.020
Total		8219093	1052092	100.000