

Sample Name : M2e, human
 Cat. No. :RP20206
 Lot. No. :PE8871805

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

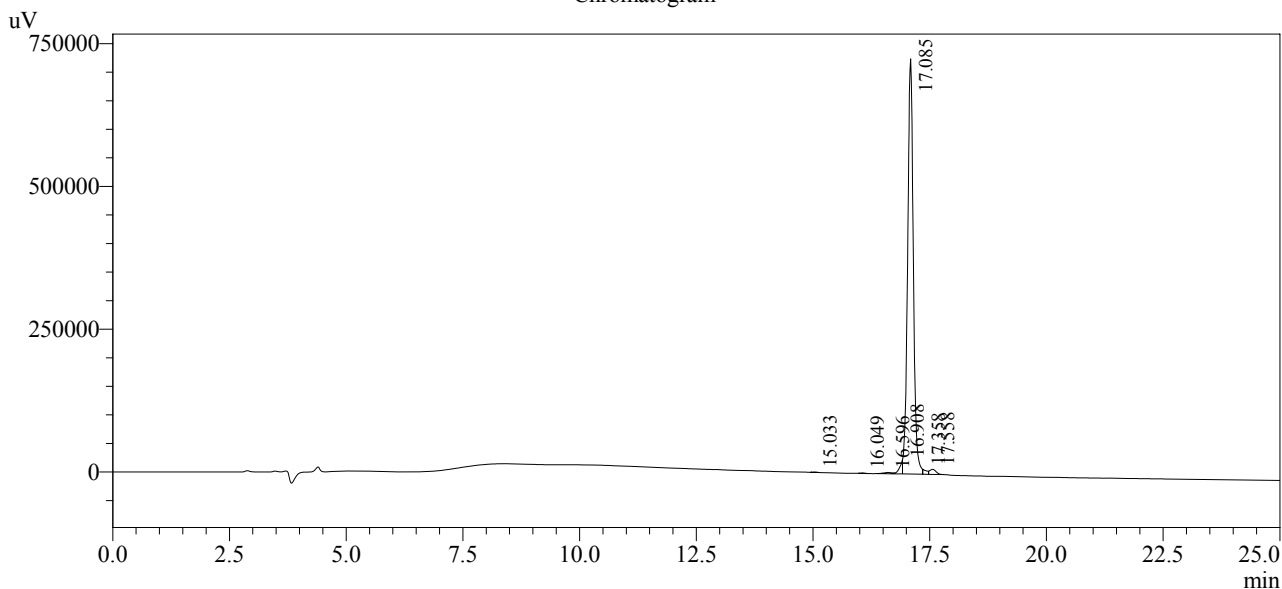

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	15.033	2528	465	0.039
2	16.049	3748	684	0.058
3	16.596	28245	1929	0.439
4	16.908	100404	21931	1.562
5	17.085	6162303	727008	95.875
6	17.358	48643	8126	0.757
7	17.558	81564	8831	1.269
Total		6427435	768974	100.000