

Sample Name :Gly-Arg-Gly-Asp-Ser
 Cat No: RP10848
 Lot No : E0671221A
 Time Processed :11:16:22 PM
 Month-Day-Year Processed :01/26/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
31.00	Pumps	B.Conc	95
31.01	Pumps	B.Conc	5
40.00	Pumps	B.Conc	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010140

<Chromatogram>

mV

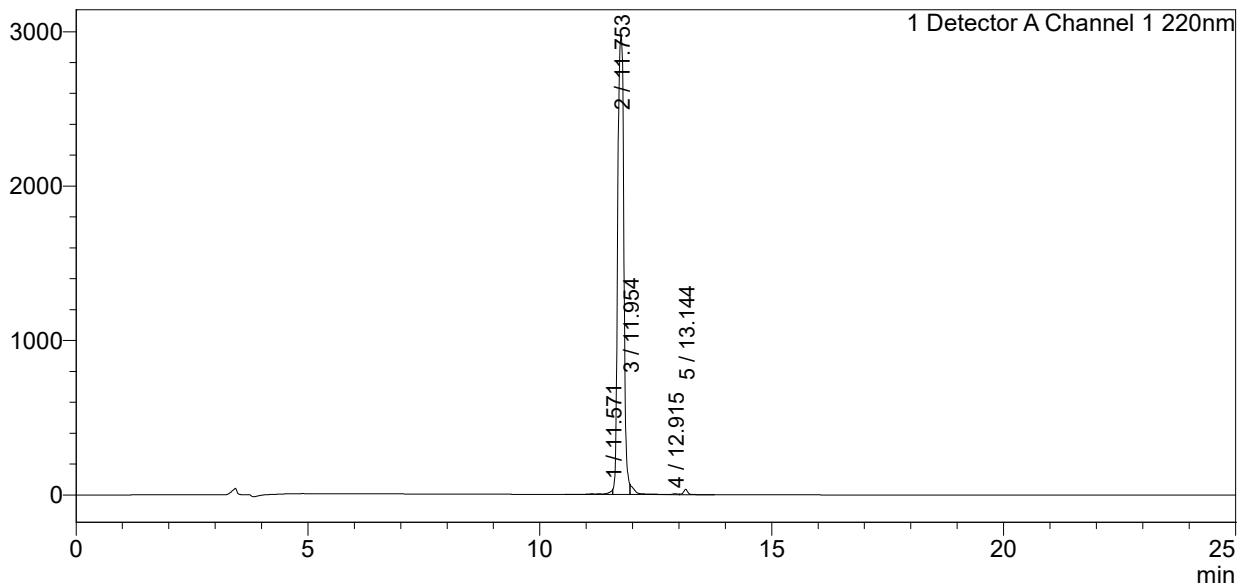

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.571	232845	29429	0.830
2	11.753	27121571	2971872	96.623
3	11.954	387499	60439	1.381
4	12.915	106189	5567	0.378
5	13.144	221309	34398	0.788
Total		28069413	3101706	100.000