

Sample Name :SIYRY  
 Cat No. :RP20234  
 Lot No. :E4850219I  
 Time Processed :10:14:40  
 Month-Day-Year Processed :09/19/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ17010507

<Chromatogram>

mV

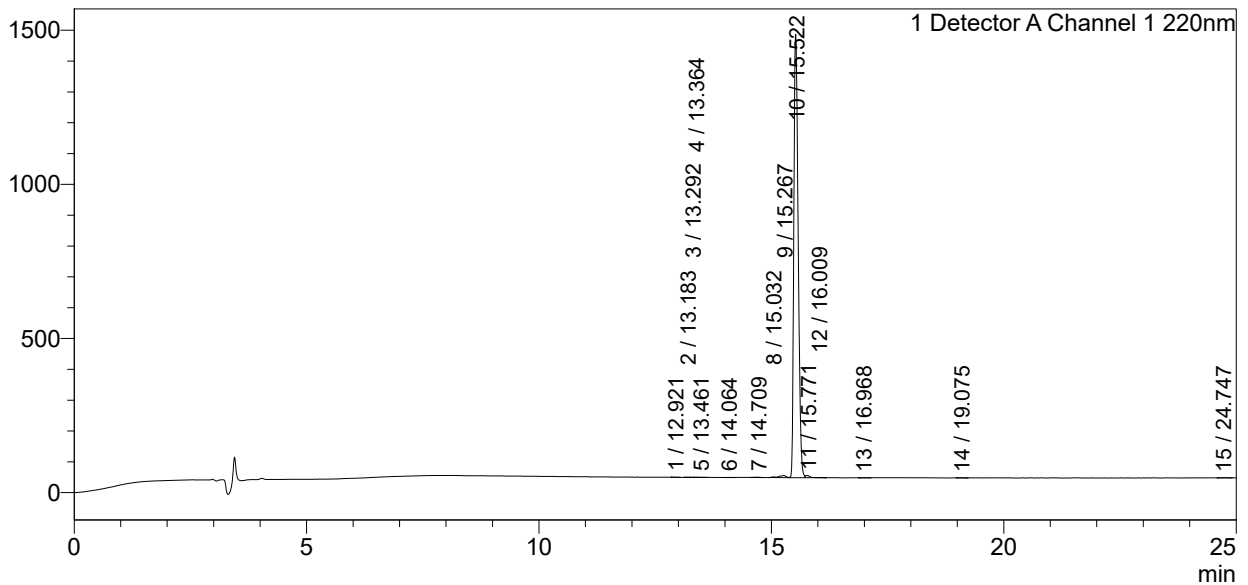

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.921	1528	349	0.016
2	13.183	1591	317	0.017
3	13.292	1277	411	0.013
4	13.364	1622	446	0.017
5	13.461	3813	584	0.040
6	14.064	3397	556	0.036
7	14.709	12621	1321	0.133
8	15.032	13306	2429	0.140
9	15.267	65729	6812	0.692
10	15.522	9328529	1437438	98.267
11	15.771	42310	7035	0.446
12	16.009	3973	467	0.042
13	16.968	3915	541	0.041
14	19.075	3609	505	0.038
15	24.747	5817	750	0.061

Peak#	Ret. Time	Area	Height	Area%
Total		9493039	1459960	100.000