

Sample Name :Neuromedin B  
 Cat No. :RP10507  
 Lot No. :E4749419I  
 Time Processed :9:43:34  
 Month-Day-Year Processed :09/19/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ17010507

<Chromatogram>

mV

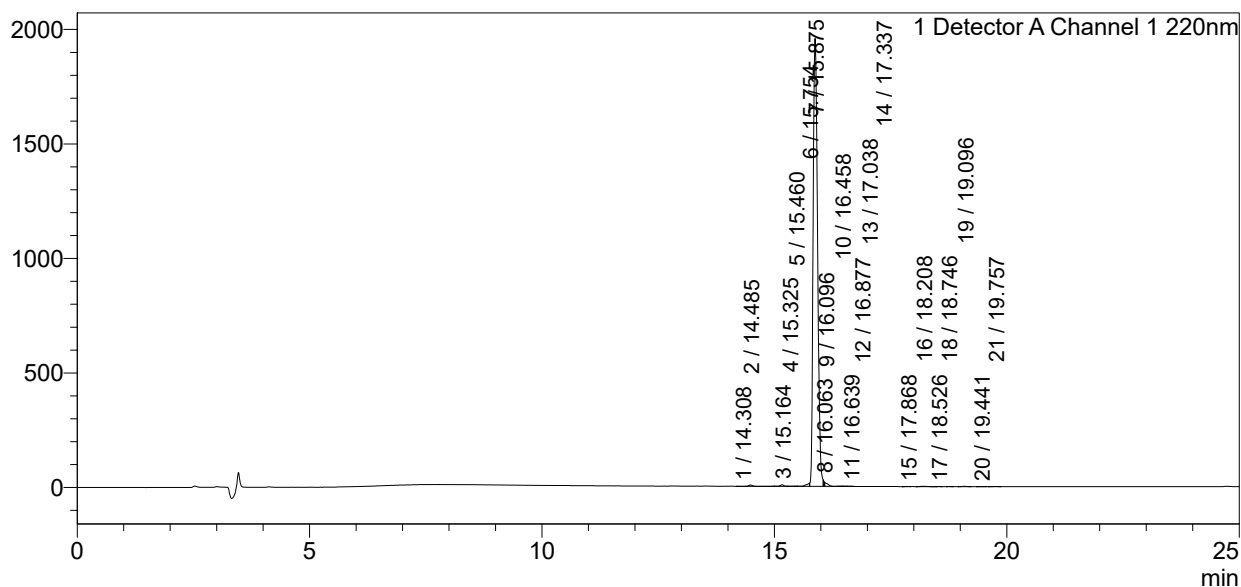

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.308	1426	250	0.011
2	14.485	35525	5691	0.268
3	15.164	38393	6458	0.289
4	15.325	5010	737	0.038
5	15.460	1992	582	0.015
6	15.754	71370	12714	0.538
7	15.875	12951682	1955454	97.596
8	16.063	41324	24317	0.311
9	16.096	73800	15710	0.556
10	16.458	3323	589	0.025
11	16.639	8066	1392	0.061
12	16.877	1052	227	0.008
13	17.038	2769	415	0.021
14	17.337	3947	624	0.030
15	17.868	2879	602	0.022

Peak#	Ret. Time	Area	Height	Area%
16	18.208	11768	1751	0.089
17	18.526	1002	228	0.008
18	18.746	1470	284	0.011
19	19.096	7318	1273	0.055
20	19.441	1520	236	0.011
21	19.757	5114	632	0.039
Total		13270749	2030166	100.000