

Sample Name :CLIP (86-100)
Cat. No. :RP20279
Lot. No. :E1276420J
Time Processed :12:23:02 PM
Month-Day-Year Processed :10/30/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
31.00	Pumps	B.Conc	95
31.01	Pumps	B.Conc	5
40.00	Pumps	B.Conc	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
Equipment: ZJ19010140

<Chromatogram>

mV

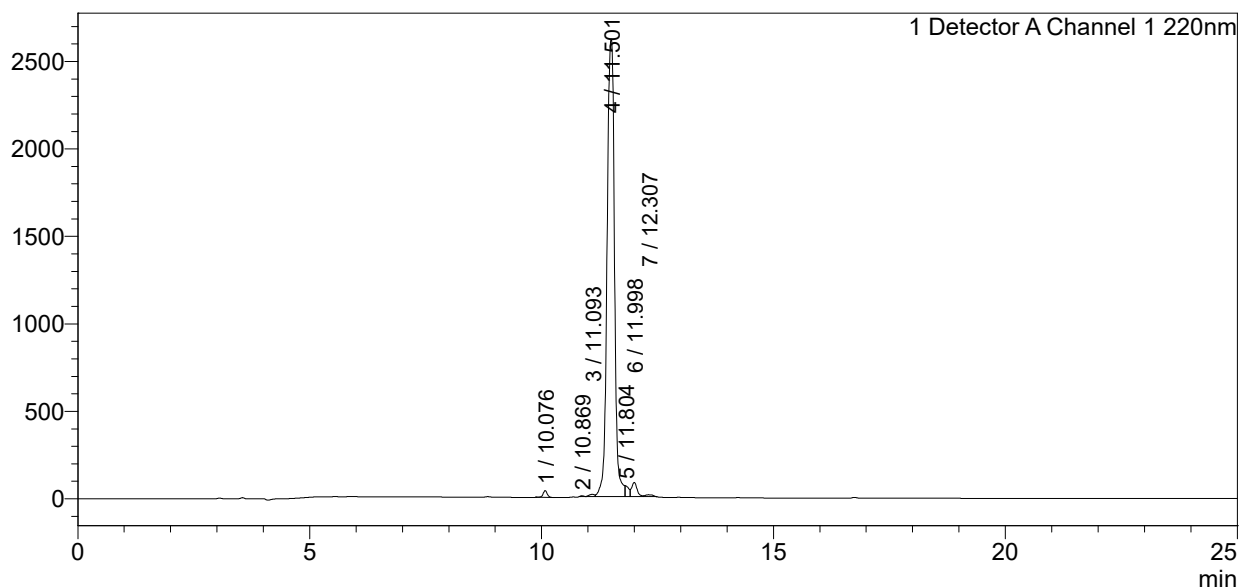

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.076	243656	38887	0.799
2	10.869	19980	4511	0.066
3	11.093	105190	12286	0.345
4	11.501	29013638	2615943	95.128
5	11.804	334584	62094	1.097
6	11.998	663115	81515	2.174
7	12.307	119410	10515	0.392
Total		30499573	2825750	100.000