

Sample Name : [Met⁵]-Enkephalin
 Cat. No. : RP10886
 Lot. No. : E1243020I

Time Processed : 6:16:49

Month-Day-Year Processed : 09/20/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow: 1 ml/min

Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: ZJ19010324

<Chromatogram>

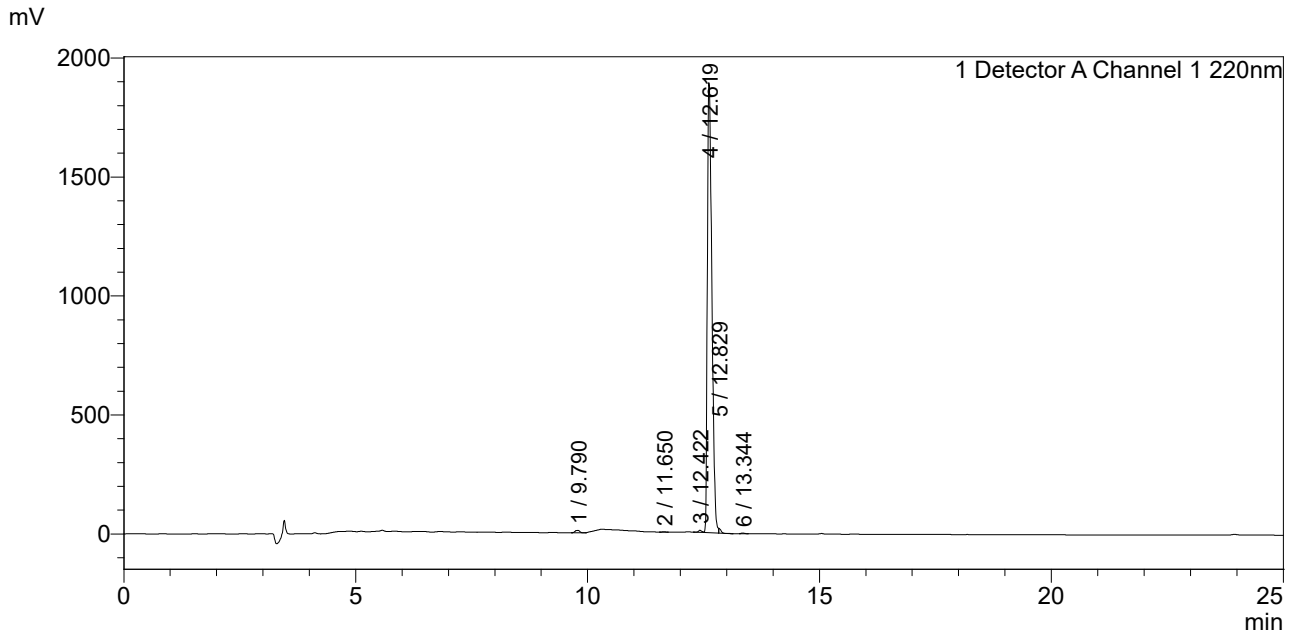

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.790	66070	9939	0.506
2	11.650	7309	1681	0.056
3	12.422	46039	8784	0.352
4	12.619	12875155	1892162	98.514
5	12.829	62758	20468	0.480
6	13.344	12066	2847	0.092
Total		13069397	1935880	100.000