


Mass Spectrum

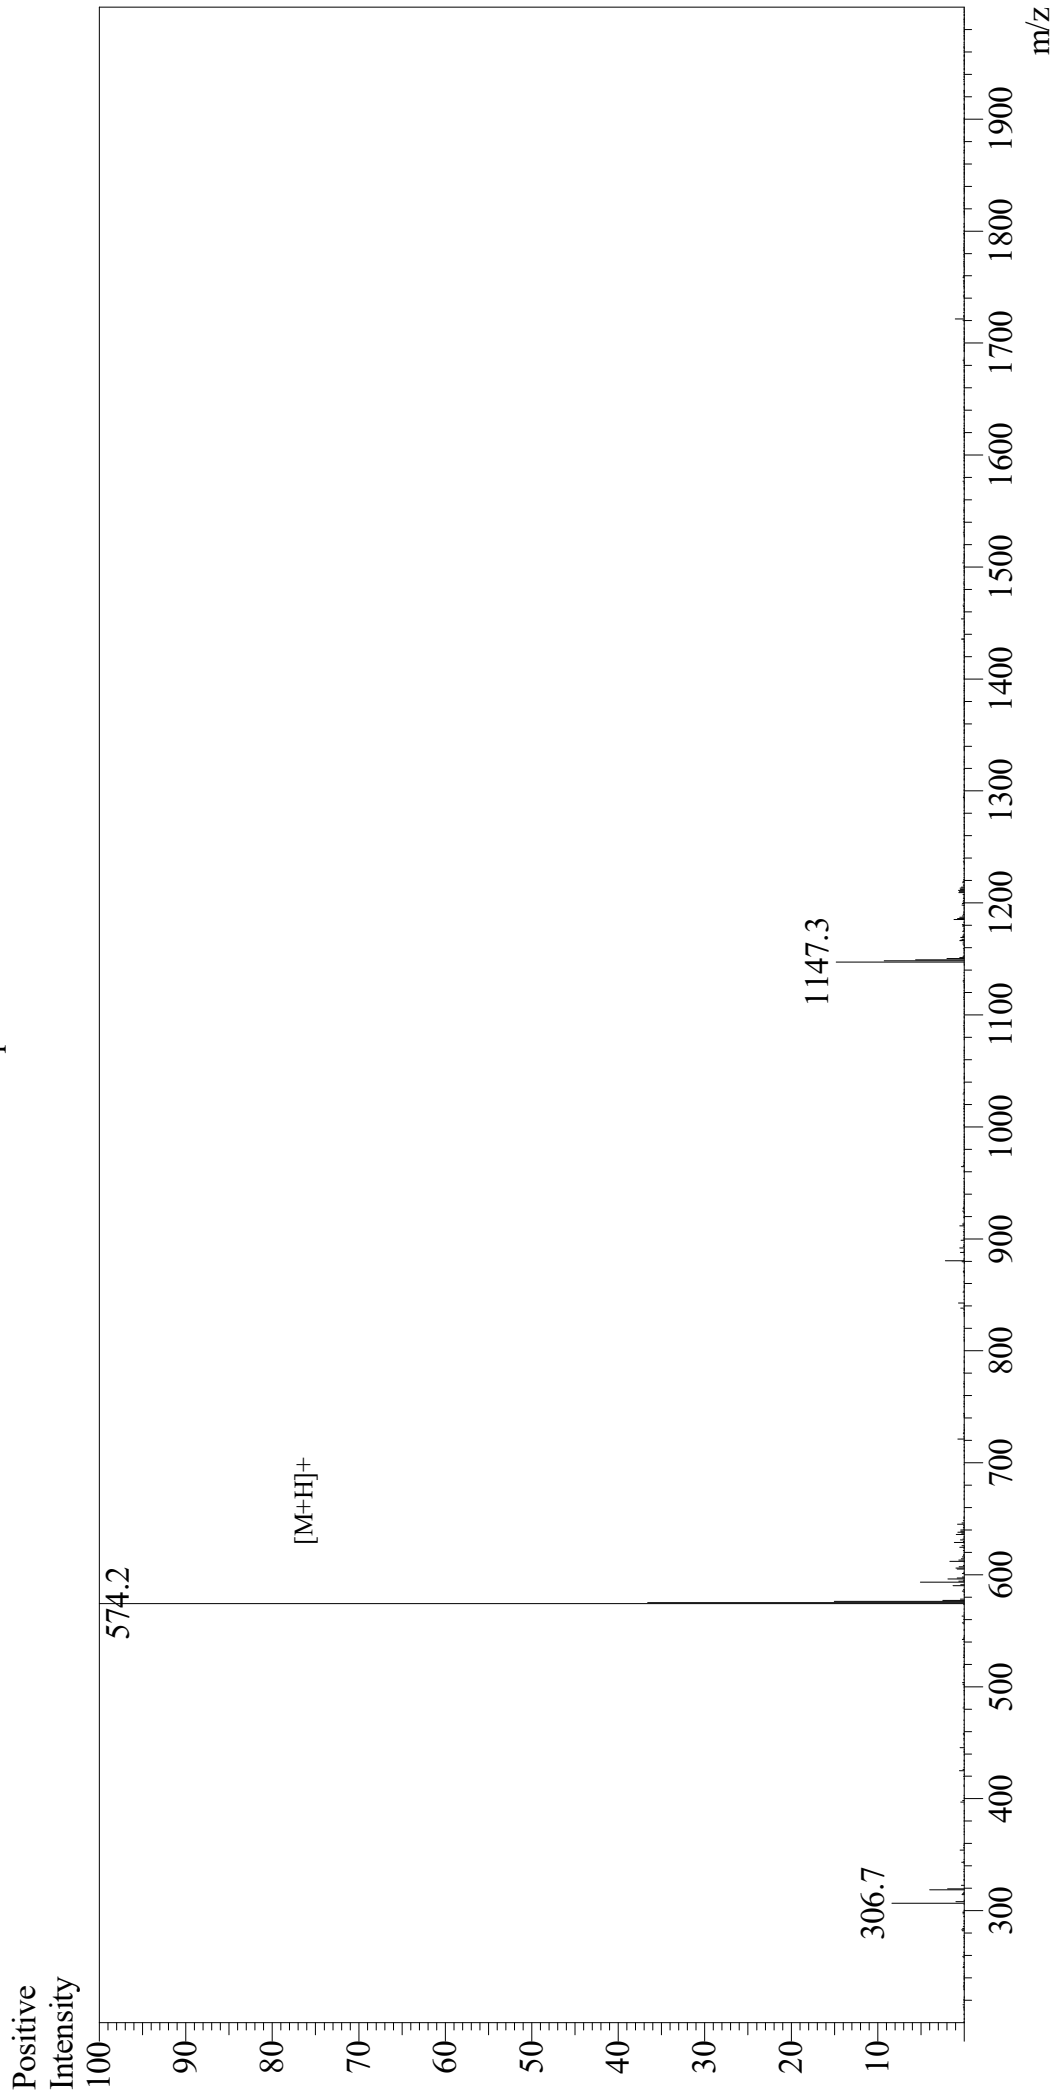

Sample Information
Month-Day Processed : 09/20/20
Time Processed : 05:50:14 PM
Injection Volume : 0.3
Sample Name : [Met⁵]-Enkephalin
Cat No. : RP10886
Lot No. : E12430201
Theoretical MW : 573.66
Observed MW : 573.2

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH