

Sample Name : DYKDDDDK Peptide
 Cat. No. : RP10586
 Lot. No. : E8668820B
 Time Processed : 10:09:25
 Month-Day-Year Processed : 03/04/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GR11010440

Chromatogram

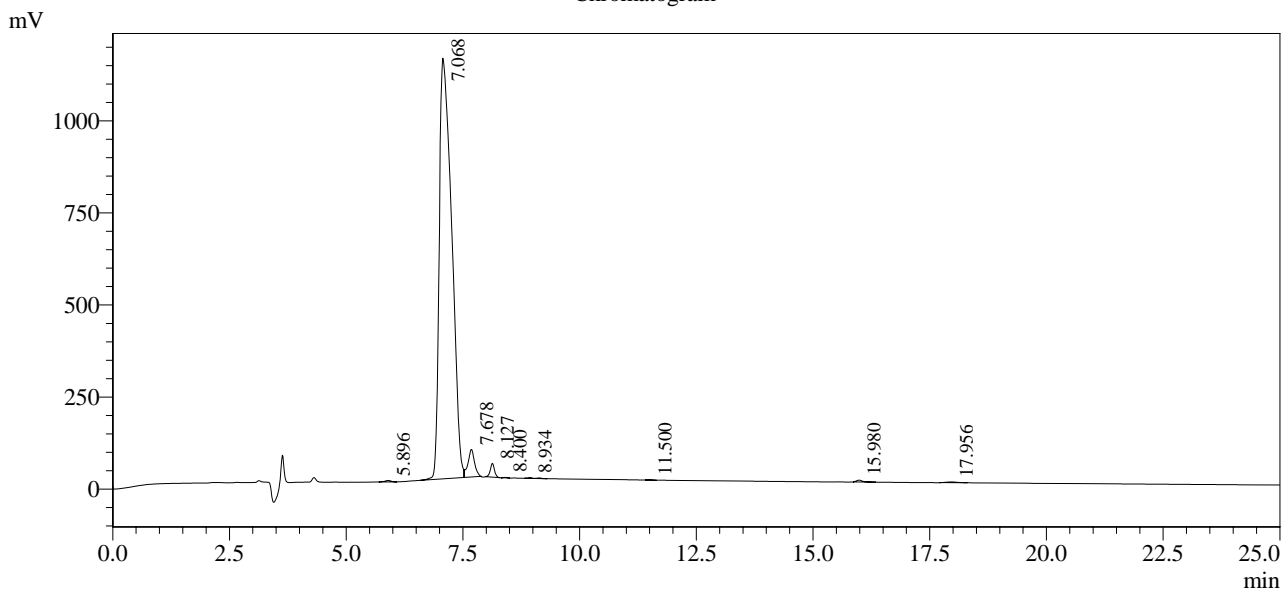

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	5.896	35108	3794	0.158
2	7.068	21122505	1142161	95.033
3	7.678	735335	75096	3.308
4	8.127	226681	37235	1.020
5	8.400	6843	1415	0.031
6	8.934	20995	1937	0.094
7	11.500	2237	418	0.010
8	15.980	45173	5084	0.203
9	17.956	31644	1969	0.142
Total		22226523	1269110	100.000