

Sample Name : CEF7, Influenza Virus NP (380-388)
 Cat. No. : RP20419
 Lot. No. : E4050121F
 Time Processed : 2:37:24
 Month-Day-Year Processed : 06/18/2021
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
31.00	Pumps	B.Conc	95
31.01	Pumps	B.Conc	5
40.00	Pumps	B.Conc	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment : ZJ19010140

<Chromatogram>

mV

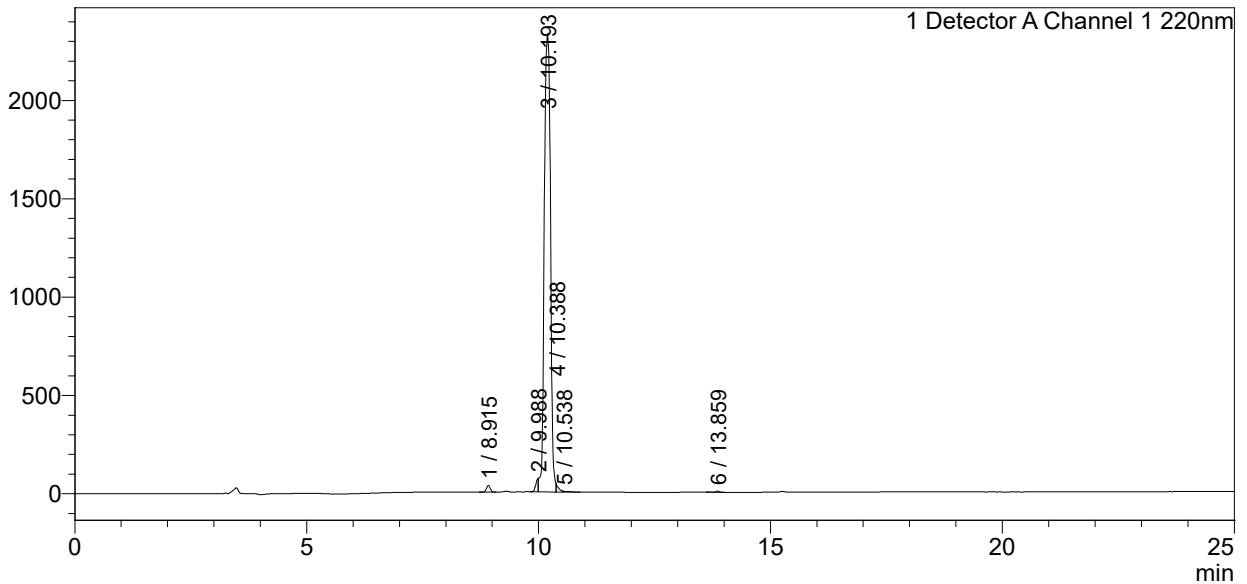

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.915	191505	33363	0.862
2	9.988	254067	66550	1.144
3	10.193	21544217	2330610	97.030
4	10.388	145545	37107	0.655
5	10.538	36196	3801	0.163
6	13.859	32225	5472	0.145
Total		22203755	2476904	100.000