

Sample Name :TFLLR
 Cat. No. : RP20354
 Lot. No. :PE9501810
 Time Processed :18:04:23
 Month-Day-Year Processed :10/31/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment :SS-CM-0310

Chromatogram

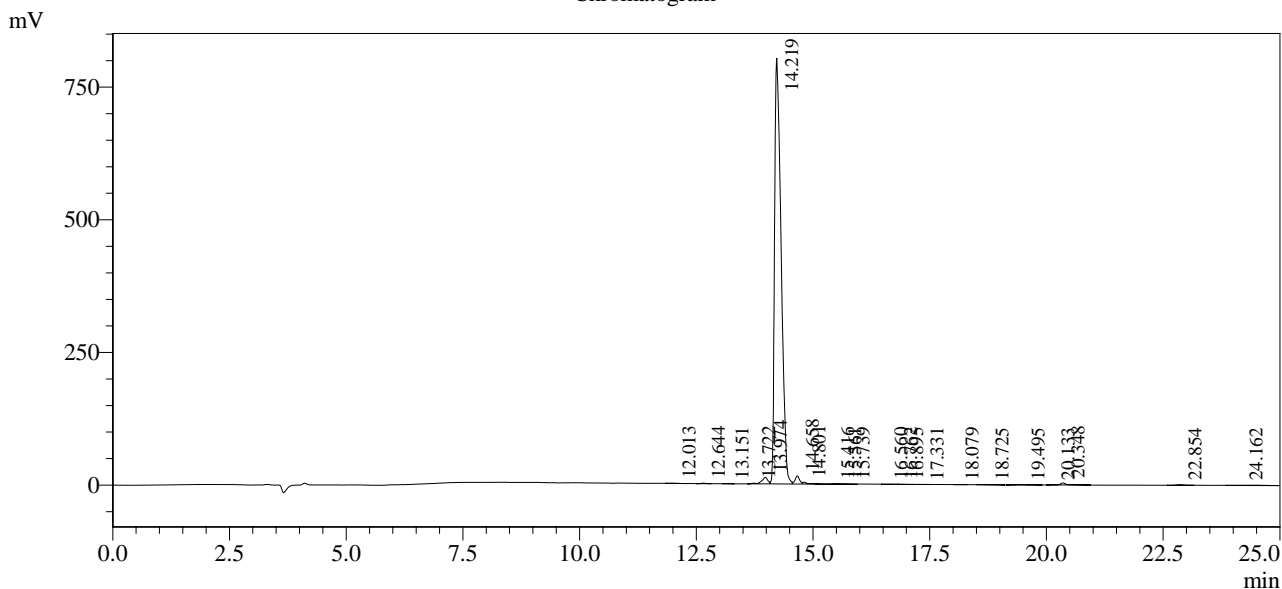

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.013	6504	645	0.080
2	12.644	5119	911	0.063
3	13.151	1026	144	0.013
4	13.722	8181	1332	0.100
5	13.974	104574	12472	1.283
6	14.219	7774661	802268	95.411
7	14.658	102984	15274	1.264
8	14.801	27725	3317	0.340
9	15.416	3047	429	0.037
10	15.561	5719	651	0.070
11	15.739	5303	635	0.065
12	16.560	3452	463	0.042
13	16.762	2341	275	0.029
14	16.895	4928	351	0.060
15	17.331	1562	196	0.019
16	18.079	1416	164	0.017
17	18.725	7350	394	0.090
18	19.495	11548	519	0.142
19	20.133	1743	231	0.021
20	20.348	33779	3823	0.415
21	22.854	12494	921	0.153
22	24.162	23174	906	0.284
Total		8148631	846323	100.000