

Sample Name :TAT
 Cat No. :RP12784
 Lot No. :E8665521F
 Time Processed :8:08:59
 Month-Day-Year Processed :06/24/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	0
5.00	Pumps	Solvent B Conc.	0
20.00	Pumps	Solvent B Conc.	30
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	0
40.00	Pumps	Solvent B Conc.	0
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

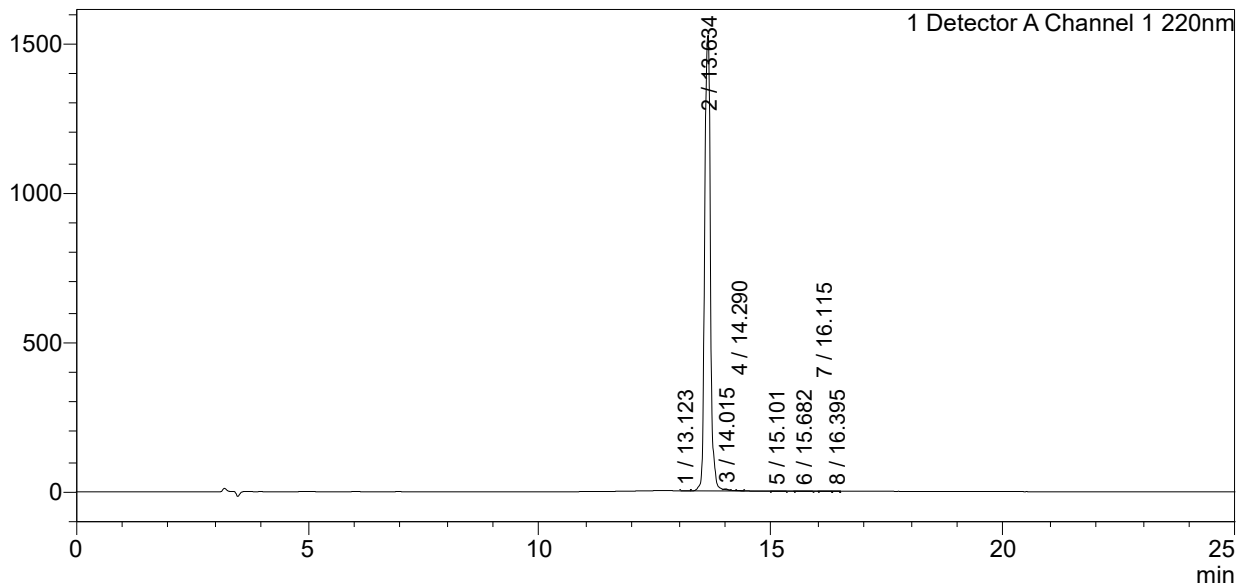

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.123	2428	543	0.019
2	13.634	13061597	1525084	99.843
3	14.015	8277	2219	0.063
4	14.290	3030	630	0.023
5	15.101	1823	204	0.014
6	15.682	3602	436	0.028
7	16.115	886	87	0.007
8	16.395	450	63	0.003
Total		13082093	1529265	100.000