

Sample Name :Fibrinogen Binding Inhibitor Peptide  
 Cat No. :RP10832  
 Lot No. :E4048719K  
 Time Processed :10:17:53 AM  
 Month-Day-Year Processed :11/18/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	5
40.00	Pumps	Solvent B Conc.	5
41.01	Controller	Stop	

<<Column Performance>>

<Detector A>  
 Column : Alltima™ C18 4.6 x 250 mm  
 Equipment:ZJ19010141

<Chromatogram>

mV

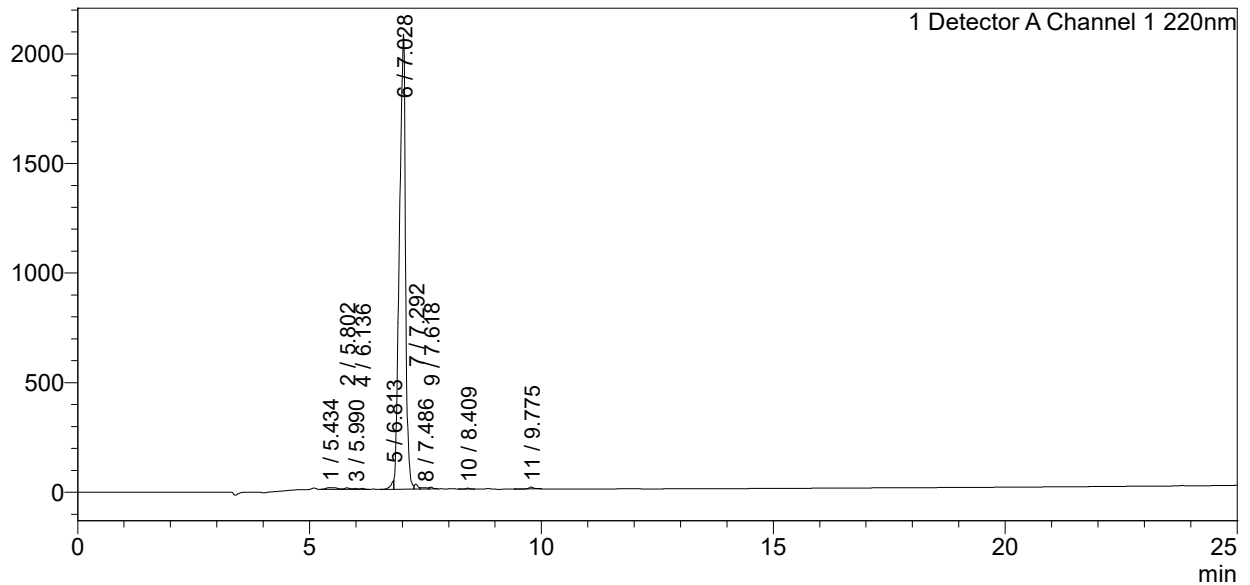

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.434	123766	7780	0.633
2	5.802	49958	6399	0.256
3	5.990	18710	3318	0.096
4	6.136	19398	3997	0.099
5	6.813	180664	37719	0.924
6	7.028	18848182	2075938	96.417
7	7.292	116093	22344	0.594
8	7.486	64856	6231	0.332
9	7.618	38952	7843	0.199
10	8.409	21485	4079	0.110
11	9.775	66453	8934	0.340
Total		19548516	2184582	100.000