

Sample Name : HPV16 E7(86-93)
 Cat. No. : RP20499
 Lot. No. : E4947820I
 Time Processed : 23:00:16
 Month-Day-Year Processed : 09/29/2020
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	0
25.00	Pumps	Pump A B.Conc	60
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	0
40.00	Pumps	Pump A B.Conc	0
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment : ZJ19010324

<Chromatogram>

mV

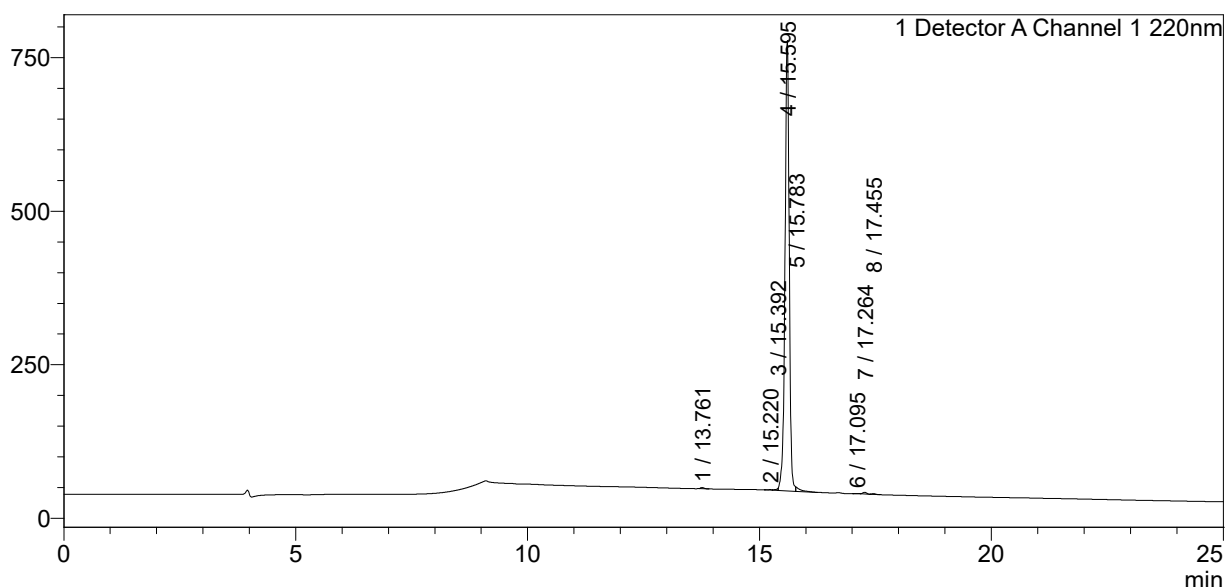

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.761	9487	1819	0.197
2	15.220	5654	894	0.117
3	15.392	12038	2867	0.250
4	15.595	4719304	733230	97.948
5	15.783	47590	7281	0.988
6	17.095	1732	378	0.036
7	17.264	15600	2840	0.324
8	17.455	6759	1327	0.140
Total		4818164	750635	100.000