

Sample Name :NP (396-404)  
 Cat No: RP20090  
 Lot No : E2658820L  
 Time Processed :0:40:12  
 Month-Day-Year Processed :12/31/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
31.00	Pumps	B.Conc	95
31.01	Pumps	B.Conc	5
40.00	Pumps	B.Conc	5
40.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010140

<Chromatogram>

mV

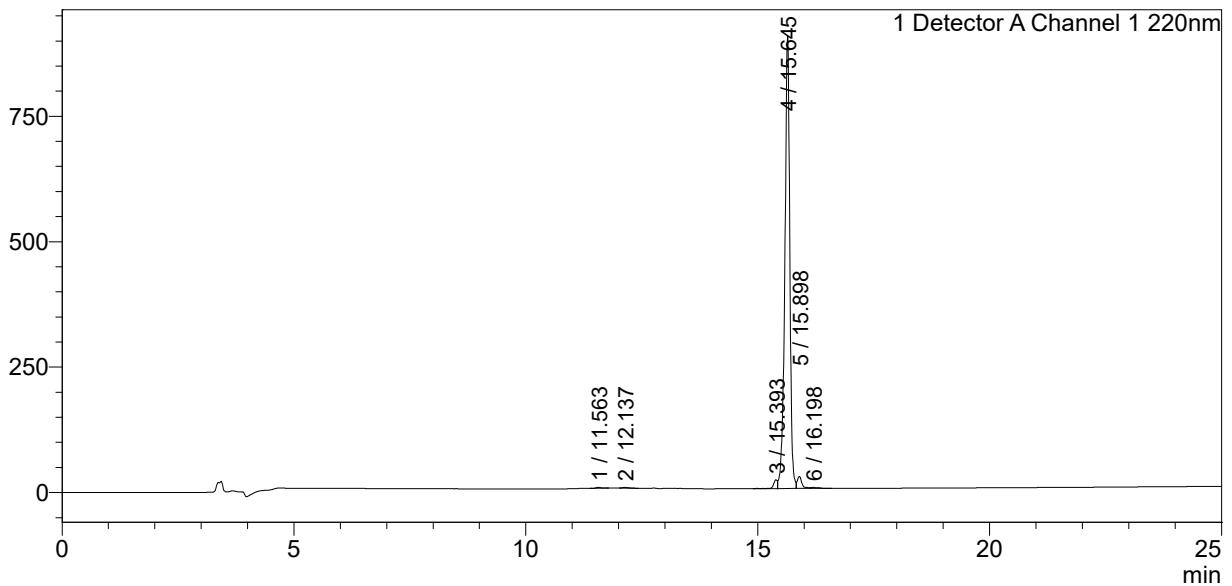

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.563	13006	1890	0.184
2	12.137	12826	1406	0.182
3	15.393	104899	17377	1.488
4	15.645	6730644	902909	95.479
5	15.898	162520	23926	2.305
6	16.198	25474	2071	0.361
Total		7049369	949581	100.000