

Sample Name : Angiotensin II (3-8), human
 Cat. No. : RP11253
 Lot. No. : PE4861812
 Time Processed : 9:53:12
 Month-Day-Year Processed : 12/30/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0309

Chromatogram

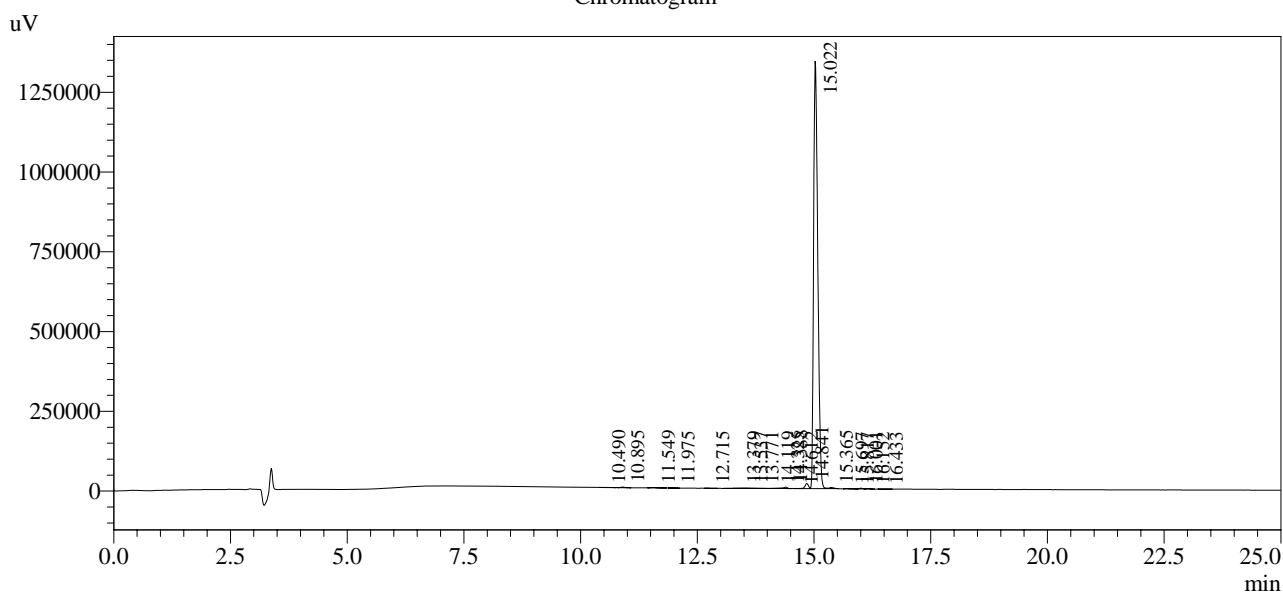

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.490	4094	403	0.048
2	10.895	10396	1874	0.121
3	11.549	9449	1117	0.110
4	11.975	2067	303	0.024
5	12.715	2793	541	0.033
6	13.379	16624	1108	0.194
7	13.537	9812	929	0.115
8	13.771	10557	741	0.123
9	14.119	3860	665	0.045
10	14.325	7352	1629	0.086
11	14.388	20678	4272	0.241
12	14.612	1295	313	0.015
13	14.841	80464	15720	0.939
14	15.022	8335379	1339753	97.304
15	15.365	24988	3737	0.292
16	15.697	3782	744	0.044
17	15.817	1576	365	0.018
18	16.001	12445	2390	0.145
19	16.152	6709	1291	0.078
20	16.433	2015	169	0.024
Total		8566334	1378064	100.000