

Sample Name :Amylin, human, amide
 Cat. No. : RP11278
 Lot. No. : PE8551905
 Time Processed : 14:28:19
 Month-Day-Year Processed : 05/28/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

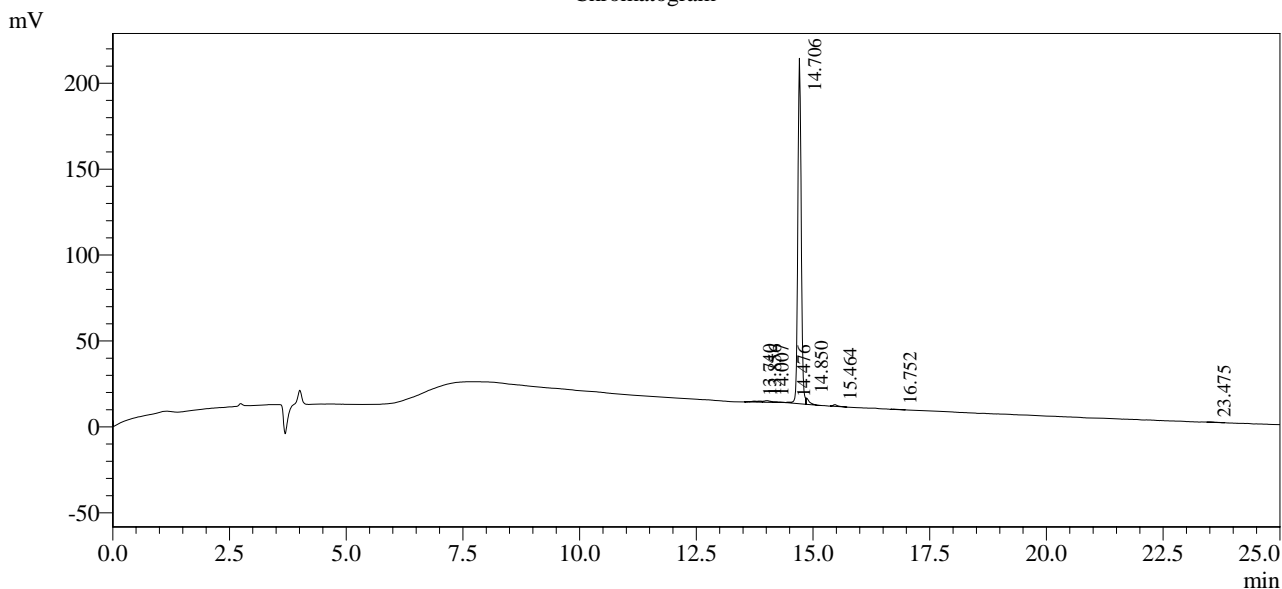

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.740	5213	594	0.486
2	13.856	4031	629	0.376
3	14.007	12316	916	1.148
4	14.476	2299	418	0.214
5	14.706	1019704	201050	95.080
6	14.850	16918	3644	1.577
7	15.464	6967	983	0.650
8	16.752	1472	197	0.137
9	23.475	3550	246	0.331
Total		1072470	208678	100.000