

Sample Name :Fibronectin Active Fragment Control  
 Cat No.: RP20347  
 Lot No.: E7071819J  
 Time Processed :10:54:35  
 Month-Day-Year Processed :10/09/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ19010324

### <Chromatogram>

mV

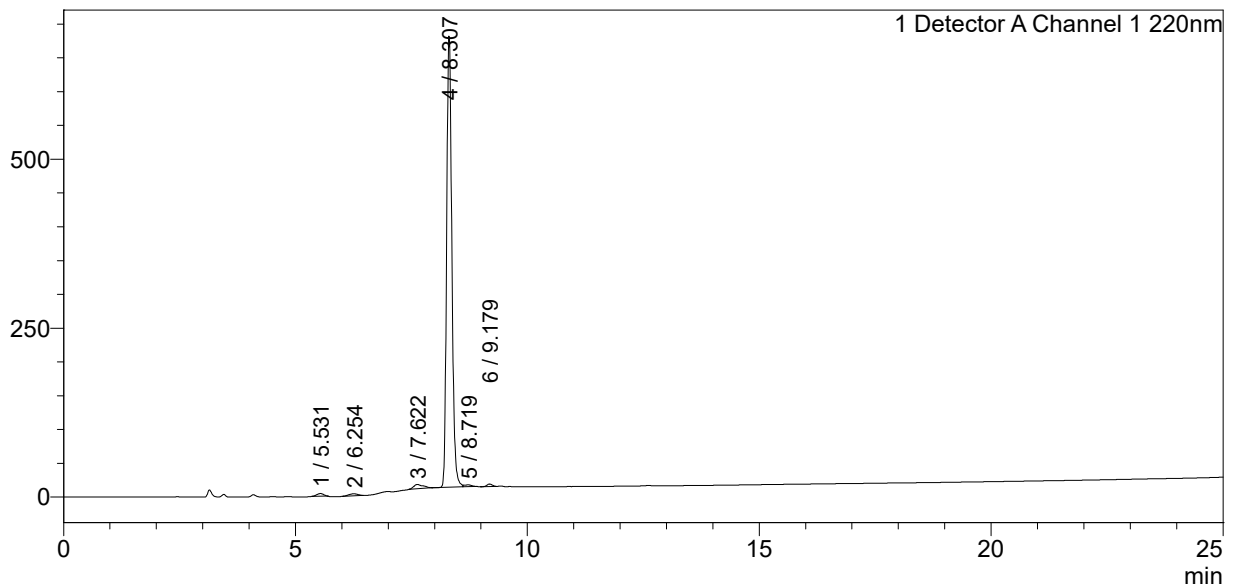

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.531	42649	4024	0.781
2	6.254	39838	2863	0.730
3	7.622	89593	6473	1.641
4	8.307	5227094	668101	95.754
5	8.719	31211	2876	0.572
6	9.179	28506	3670	0.522
Total		5458890	688006	100.000