

Sample Name :Protease-Activated Receptor-2 Activating Peptide  
 Cat No. : RP19975  
 Lot No. : E1250320G  
 Time Processed : 0:58:43  
 Month-Day-Year Processed : 07/02/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment:GK12010012

### <Chromatogram>

mV

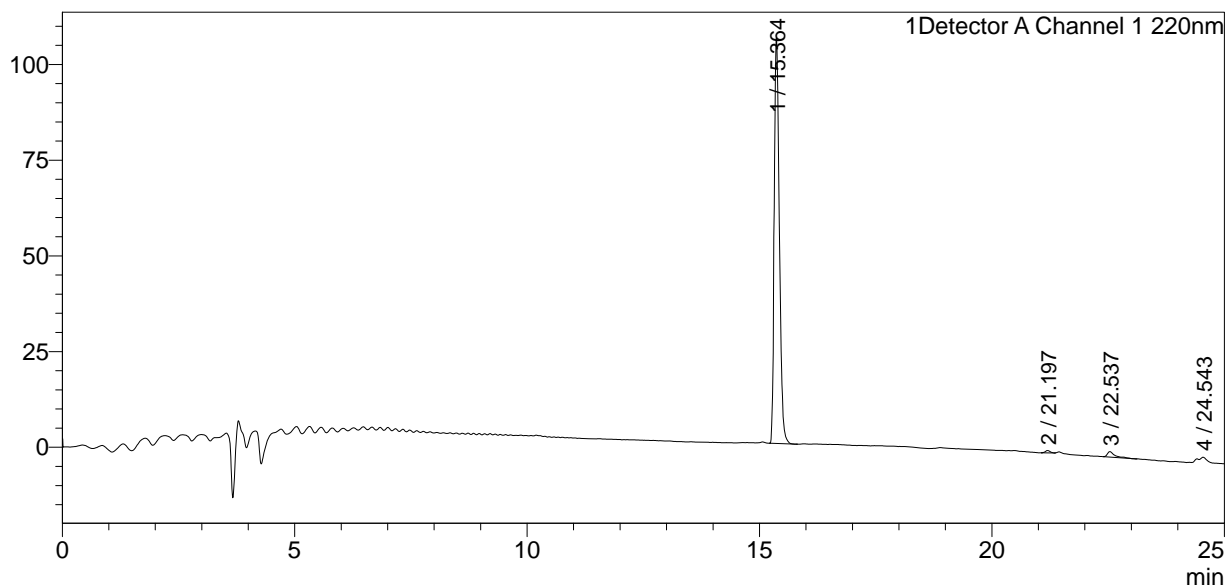

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.364	816724	105972	95.219
2	21.197	4310	610	0.502
3	22.537	15696	1411	1.830
4	24.543	20999	1502	2.448
Total		857729	109496	100.000