

Sample Name : N-Formyl-Nle-Leu-Phe-Nle-Tyr-Lys
 Cat. No. : RP12959
 Lot. No. : PE4811611

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
10.00	Pumps	Pump A B.Conc	35	
35.00	Pumps	Pump A B.Conc	95	
41.00	Pumps	Pump A B.Conc	95	
41.01	Pumps	Pump A B.Conc	5	
50.00	Pumps	Pump A B.Conc	5	
50.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

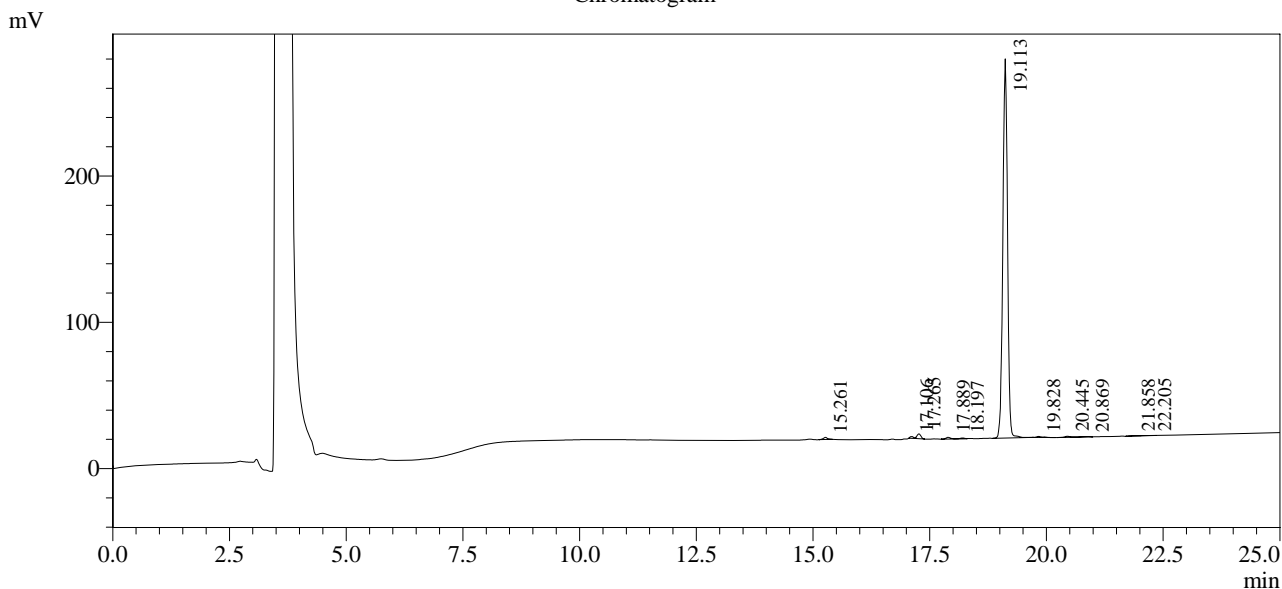

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	15.261	9050	1453	0.481
2	17.106	7567	1339	0.402
3	17.265	18354	3252	0.976
4	17.889	8247	1191	0.439
5	18.197	4725	590	0.251
6	19.113	1810673	259241	96.277
7	19.828	6269	671	0.333
8	20.445	6865	716	0.365
9	20.869	4353	375	0.231
10	21.858	1219	145	0.065
11	22.205	3368	243	0.179
Total		1880691	269217	100.000