

Sample Name : β -Amyloid (1-40), rat
 Cat No. : RP10016
 Lot No. : E1399219G
 Time Processed : 9:23:35
 Month-Day-Year Processed : 11/26/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	15	
25.00	Pumps	Pump B Conc.	75	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	15	
37.00	Pumps	Pump B Conc.	15	
37.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

Equipment: GR09010180

Chromatogram

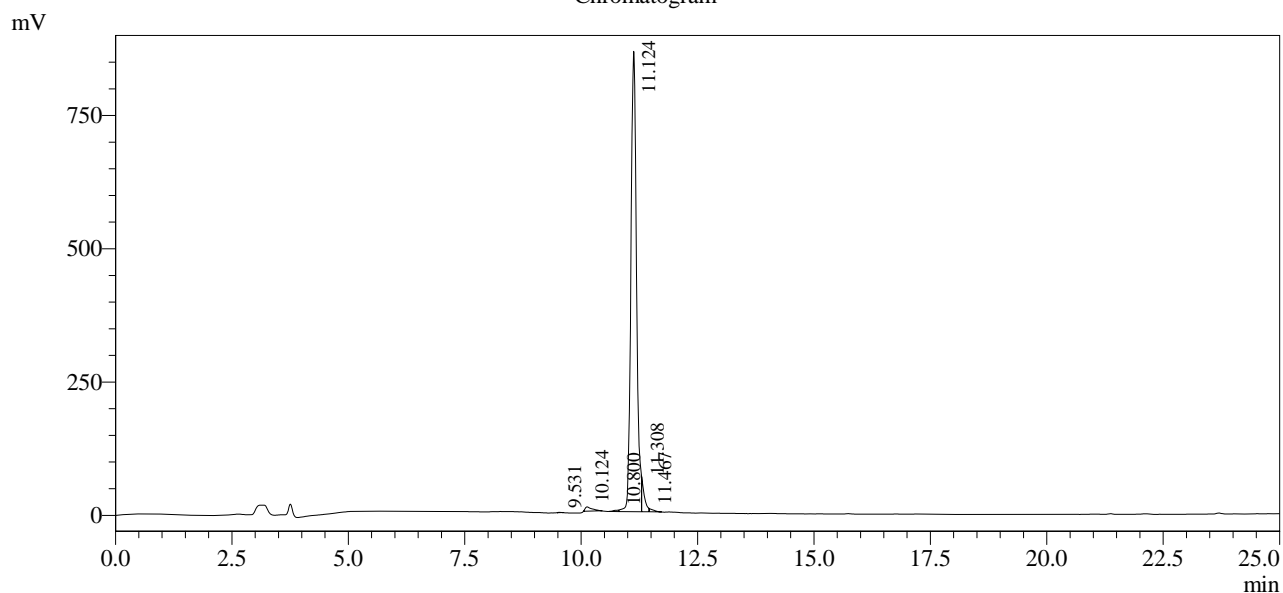

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.531	2311	577	0.030
2	10.124	83267	7958	1.091
3	10.800	18647	2636	0.244
4	11.124	7257361	863597	95.129
5	11.308	231147	59688	3.030
6	11.467	36217	6036	0.475
Total		7628950	940493	100.000