

Sample Name :C-Peptide, dog
 Cat. No. : RP11115
 Lot. No. : E7291519H
 Time Processed :12:42:52
 Month-Day-Year Processed :09/01/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

| Time | Unit | Command | Value | Comment |
|-------|------------|--------------|-------|---------|
| 0.01 | Pumps | Pump B Conc. | 5 | |
| 25.00 | Pumps | Pump B Conc. | 65 | |
| 25.01 | Pumps | Pump B Conc. | 95 | |
| 27.00 | Pumps | Pump B Conc. | 95 | |
| 27.01 | Pumps | Pump B Conc. | 5 | |
| 35.00 | Pumps | Pump B Conc. | 5 | |
| 35.01 | Controller | Stop | | |


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment :SS-CM-0310

Chromatogram

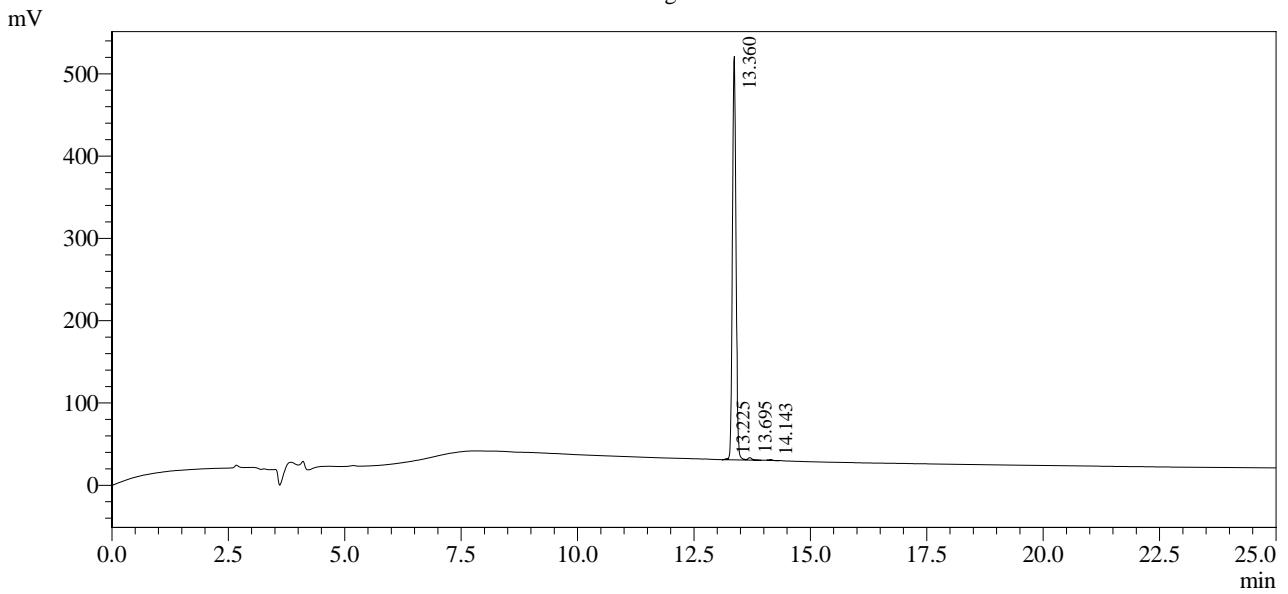

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

| Peak# | Ret. Time | Area | Height | Area % |
|-------|-----------|---------|--------|---------|
| 1 | 13.225 | 6424 | 1620 | 0.243 |
| 2 | 13.360 | 2613947 | 490122 | 98.897 |
| 3 | 13.695 | 17537 | 2929 | 0.664 |
| 4 | 14.143 | 5201 | 987 | 0.197 |
| Total | | 2643109 | 495658 | 100.000 |