

Sample Name : Bradykinin
 Cat. No. : RP11129
 Lot. No. : PE5941812
 Time Processed : 13:38:25
 Month-Day-Year Processed : 12/13/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0309

Chromatogram

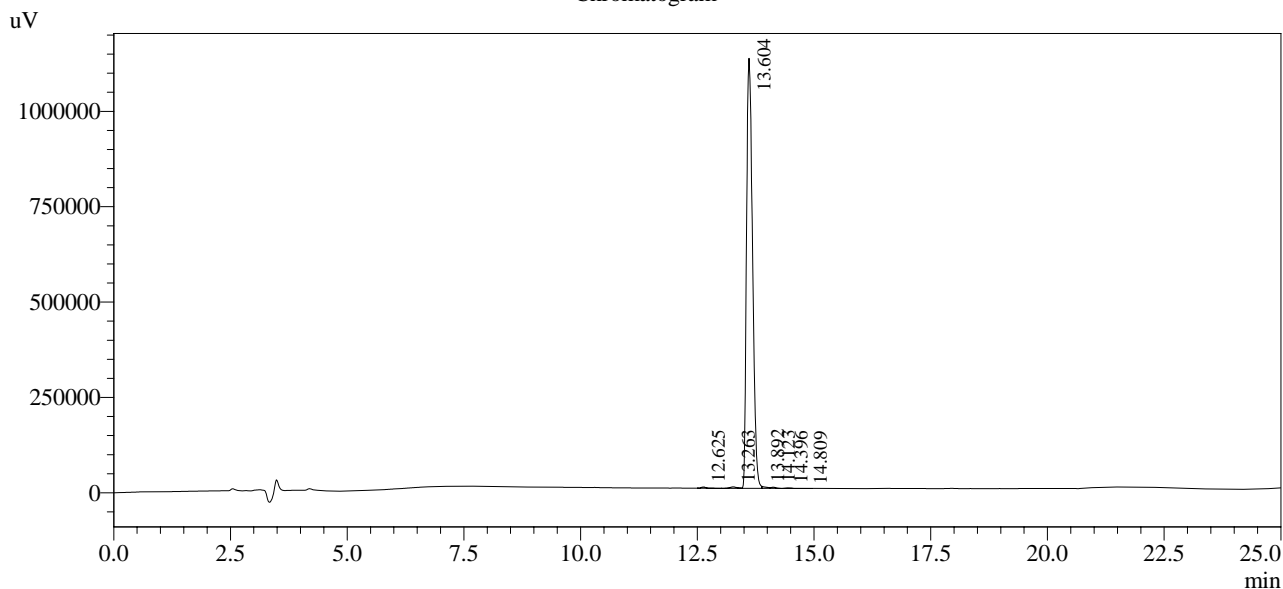

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.625	23227	3387	0.226
2	13.263	42681	3905	0.416
3	13.604	10115748	1127495	98.628
4	13.892	31950	4898	0.312
5	14.123	22000	3012	0.214
6	14.396	17568	1583	0.171
7	14.809	3301	513	0.032
Total		10256474	1144791	100.000