

Sample Name :N-Acetyl-Ser-Asp-Lys-Pro
 Cat No. :RP10555
 Lot No. :E5067220J
 Time Processed :13:42:43
 Month-Day-Year Processed :10/13/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	0
5.00	Pumps	B.Conc	0
20.00	Pumps	B.Conc	30
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	0
35.00	Pumps	B.Conc	0
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

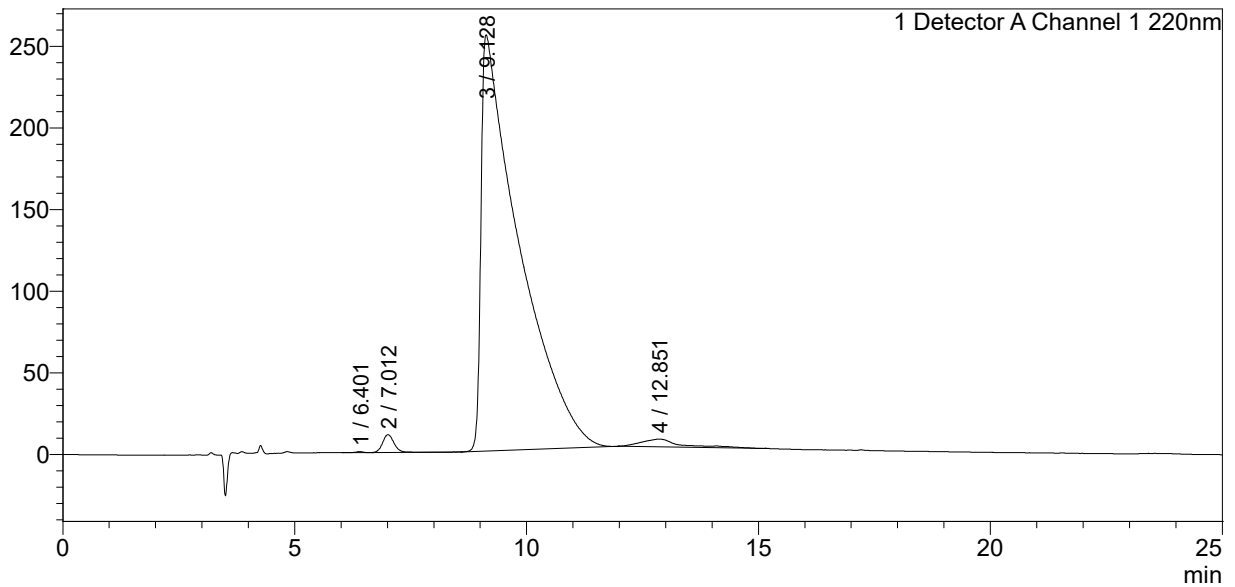

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	6.401	6064	631	0.040
2	7.012	180042	10873	1.195
3	9.128	14596614	255091	96.888
4	12.851	282679	4746	1.876
Total		15065399	271341	100.000