

Sample Name :LAH4
 Cat. No. : RP20096
 Lot. No. : E4750420K

Time Processed :4:15:26 AM
 Month-Day-Year Processed :11/12/2020
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK11010011

<Chromatogram>

mV

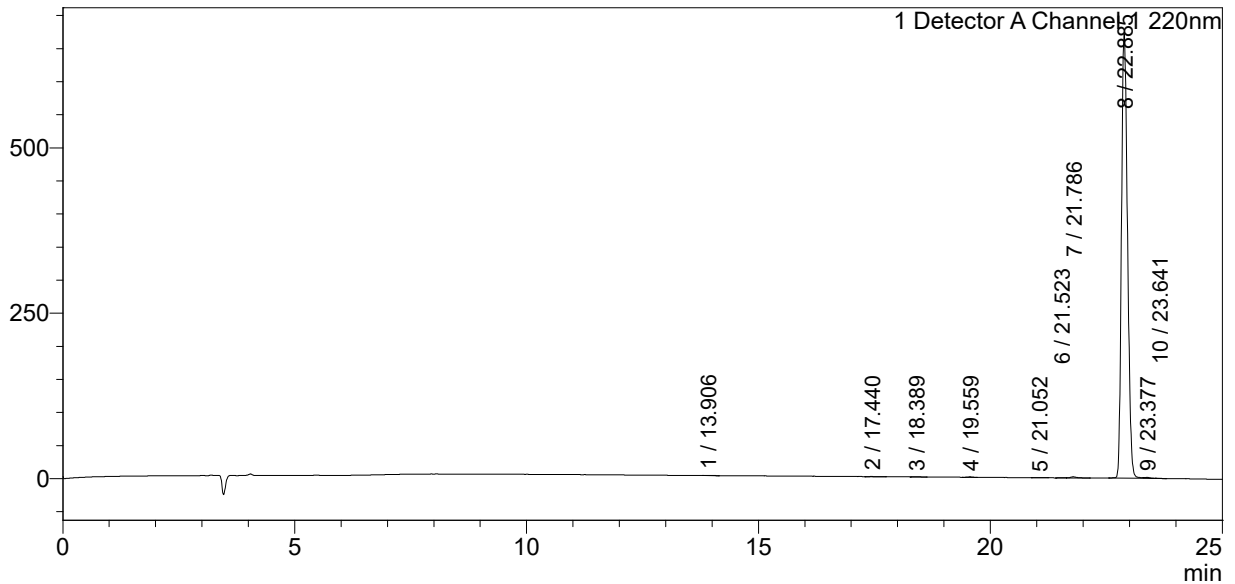

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.906	1162	131	0.019
2	17.440	1556	154	0.025
3	18.389	2407	333	0.039
4	19.559	4011	599	0.065
5	21.052	3018	294	0.049
6	21.523	3695	525	0.060
7	21.786	16032	1637	0.261
8	22.885	6101386	671981	99.372
9	23.377	5610	939	0.091
10	23.641	1063	143	0.017
Total		6139940	676735	100.000