


Mass Spectrum

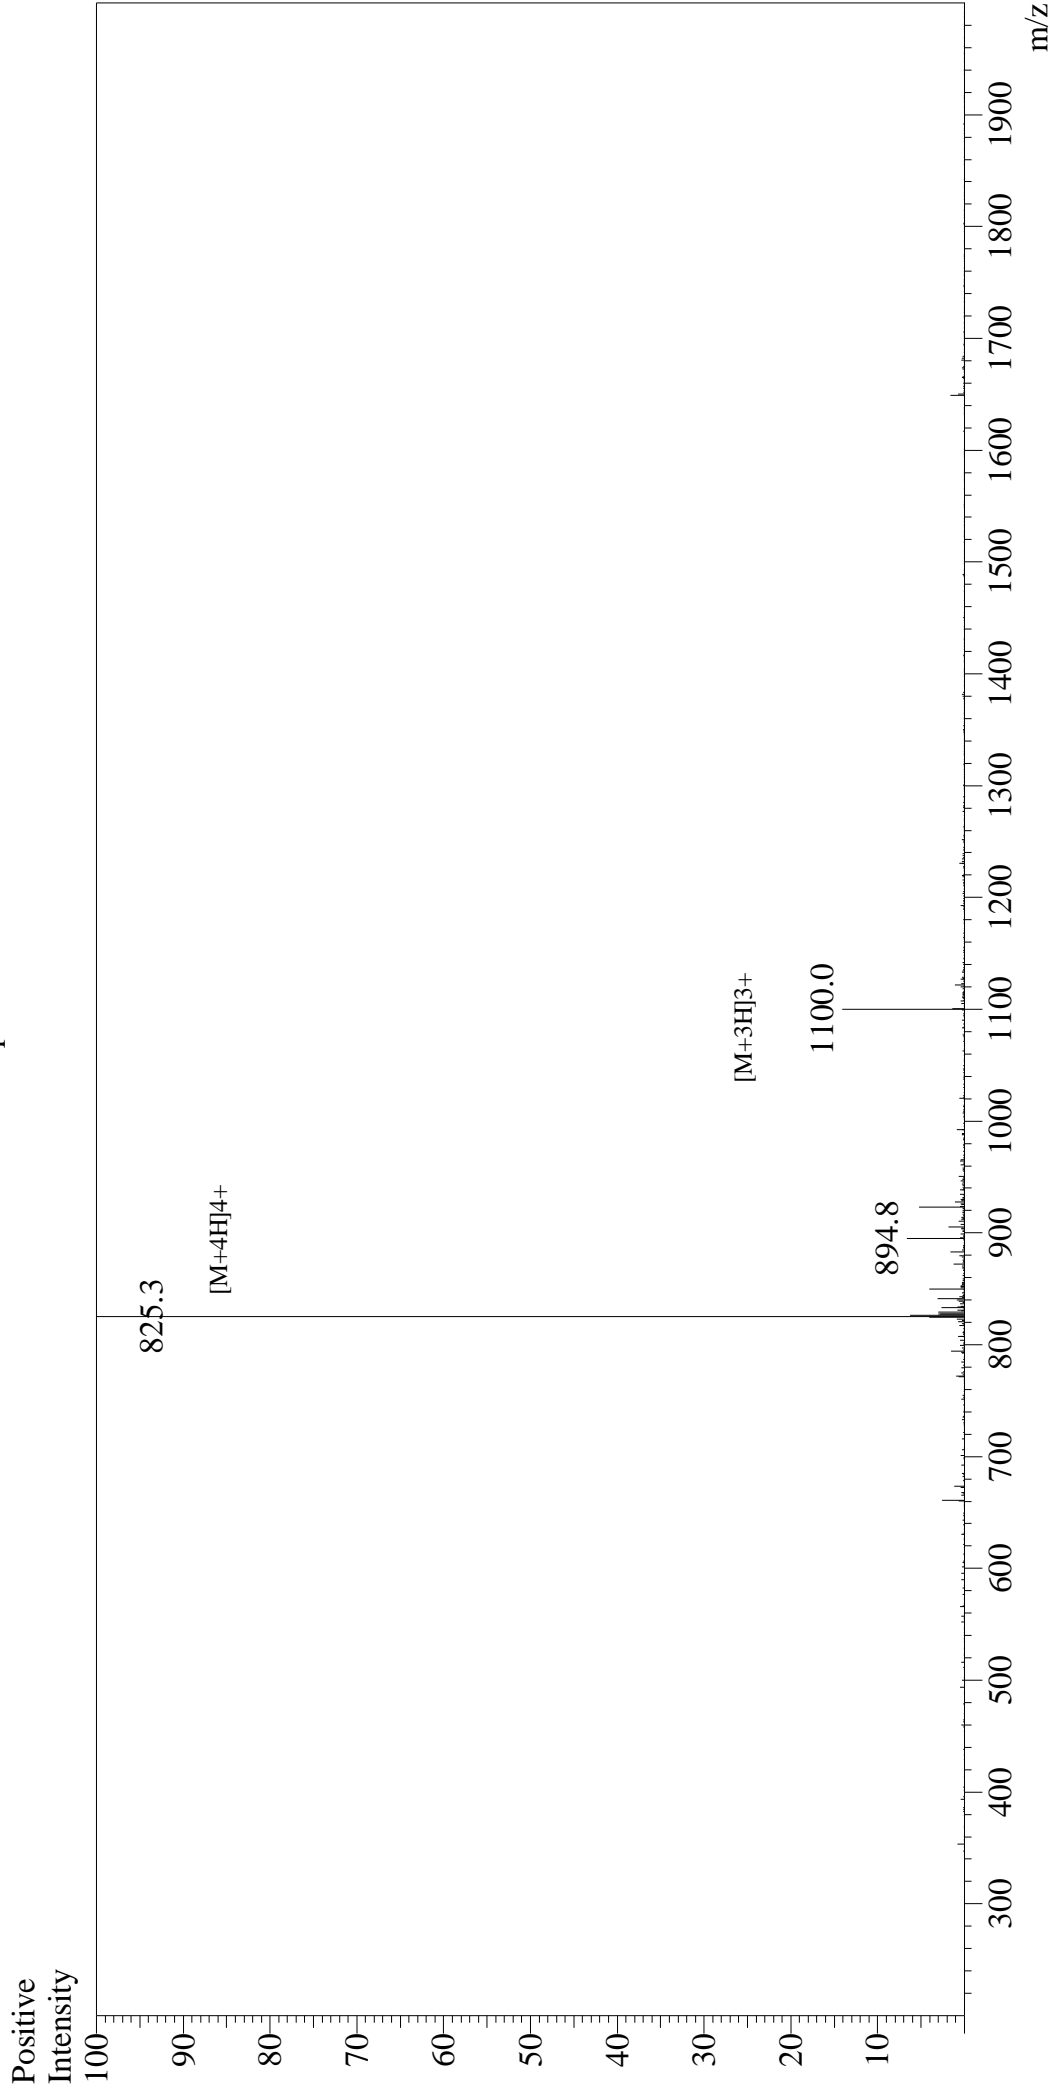

Sample Information

User : Gary
Month-Day Processed : 10/26/18
Time Processed : 18:13:57
Injection Volume : 0.2
Sample Name : GLP-1 (7-36), amide, human
Cat No. : RP10773
Lot No. : PE4731810
Theoretical MW : 3297.50
Observed MW : 3297.2

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250°C
Block Temp : 200°C

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH