

Sample Name : Colivelin
 Cat. No. : RP20167
 Lot. No. : E1701820I
 Time Processed : 7:41:38
 Month-Day-Year Processed : 09/14/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010324

<Chromatogram>

mV

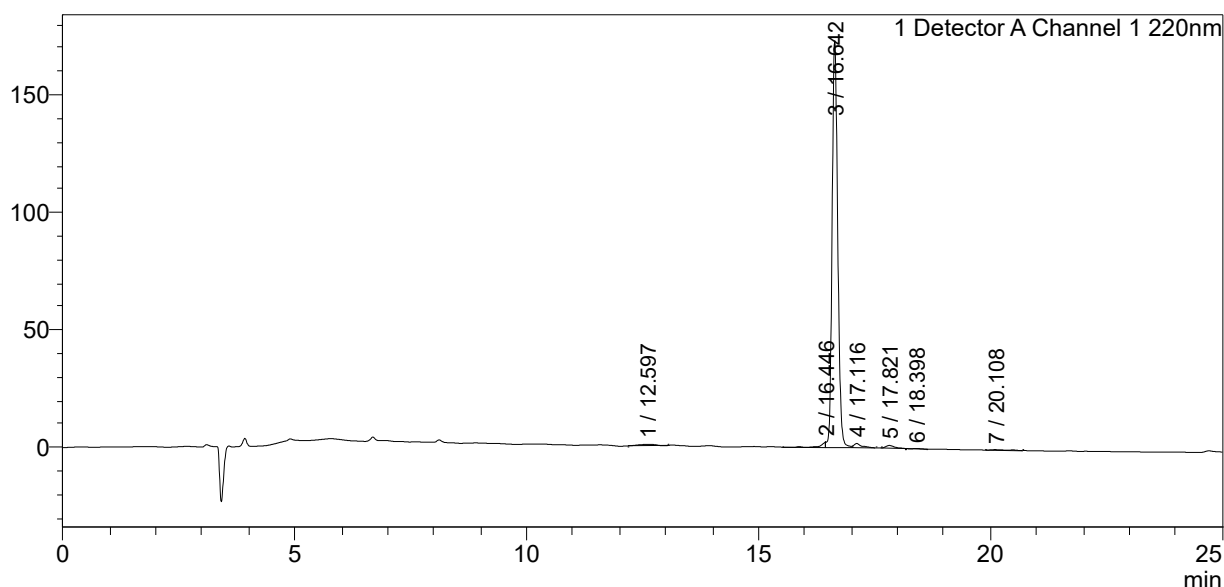

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.597	11914	533	0.778
2	16.446	19609	2147	1.280
3	16.642	1456437	173083	95.072
4	17.116	21215	1770	1.385
5	17.821	14660	1147	0.957
6	18.398	1200	157	0.078
7	20.108	6903	254	0.451
Total		1531937	179091	100.000