

Sample Name :C-Peptide (3-33), human
 Cat No. :RP11116
 Lot No. :E8066921C
 Time Processed :20:56:21
 Month-Day-Year Processed :04/08/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
10.00	Pumps	B.Conc	35
35.00	Pumps	B.Conc	95
37.00	Pumps	B.Conc	95
37.01	Pumps	B.Conc	5
45.00	Pumps	B.Conc	5
45.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

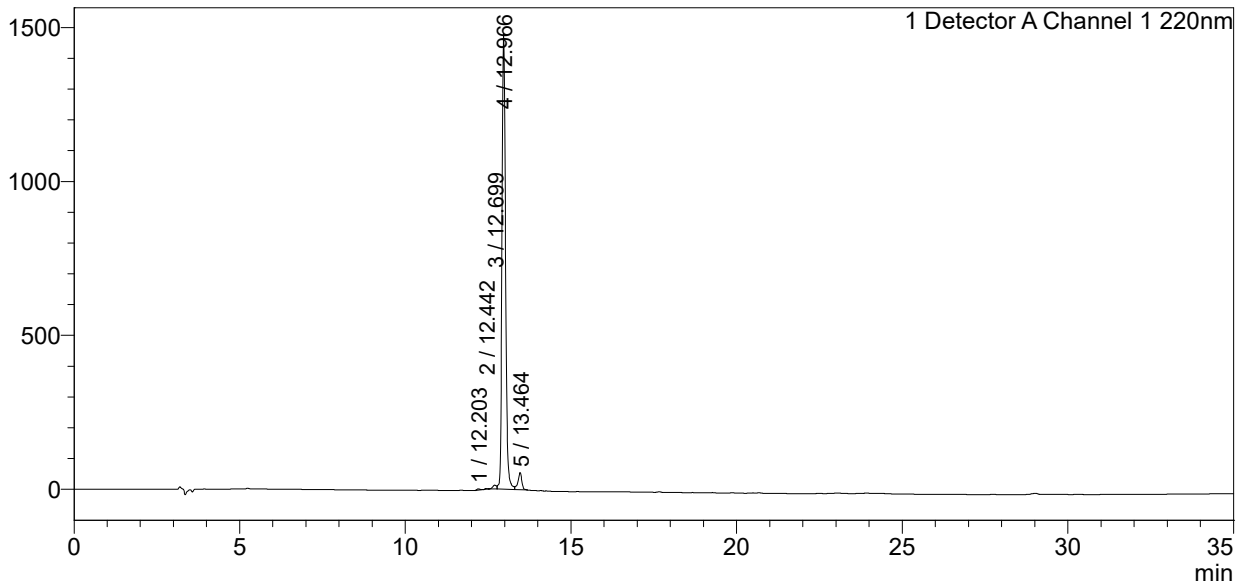

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.203	27084	3934	0.232
2	12.442	11218	2277	0.096
3	12.699	99938	12339	0.854
4	12.966	11121961	1479821	95.080
5	13.464	437272	55400	3.738
Total		11697473	1553771	100.000