

Sample Name : PLP(139-151)
 Cat No. : RP10550
 Lot No. : PE1441802

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

<Chromatogram>

mV

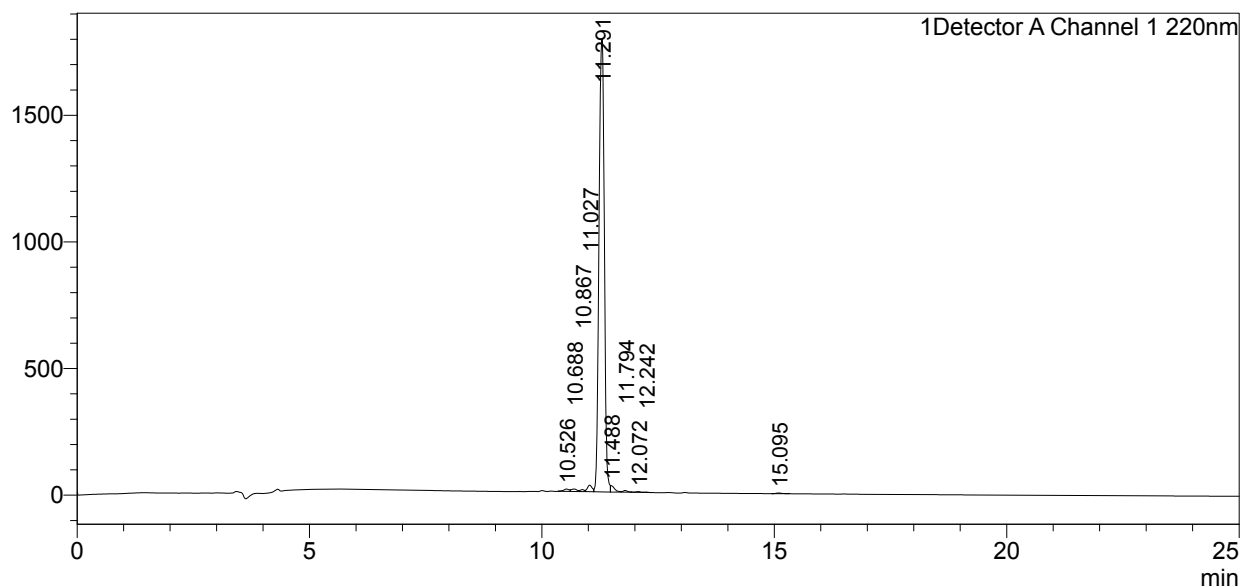

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.526	78669	9428	0.529
2	10.688	84646	9874	0.570
3	10.867	46298	7990	0.312
4	11.027	182730	25858	1.230
5	11.291	14217606	1788761	95.666
6	11.488	147697	25257	0.994
7	11.794	48876	6757	0.329
8	12.072	24585	3176	0.165
9	12.242	9034	1534	0.061
10	15.095	21595	2641	0.145
Total		14861735	1881276	100.000