


Mass Spectrum

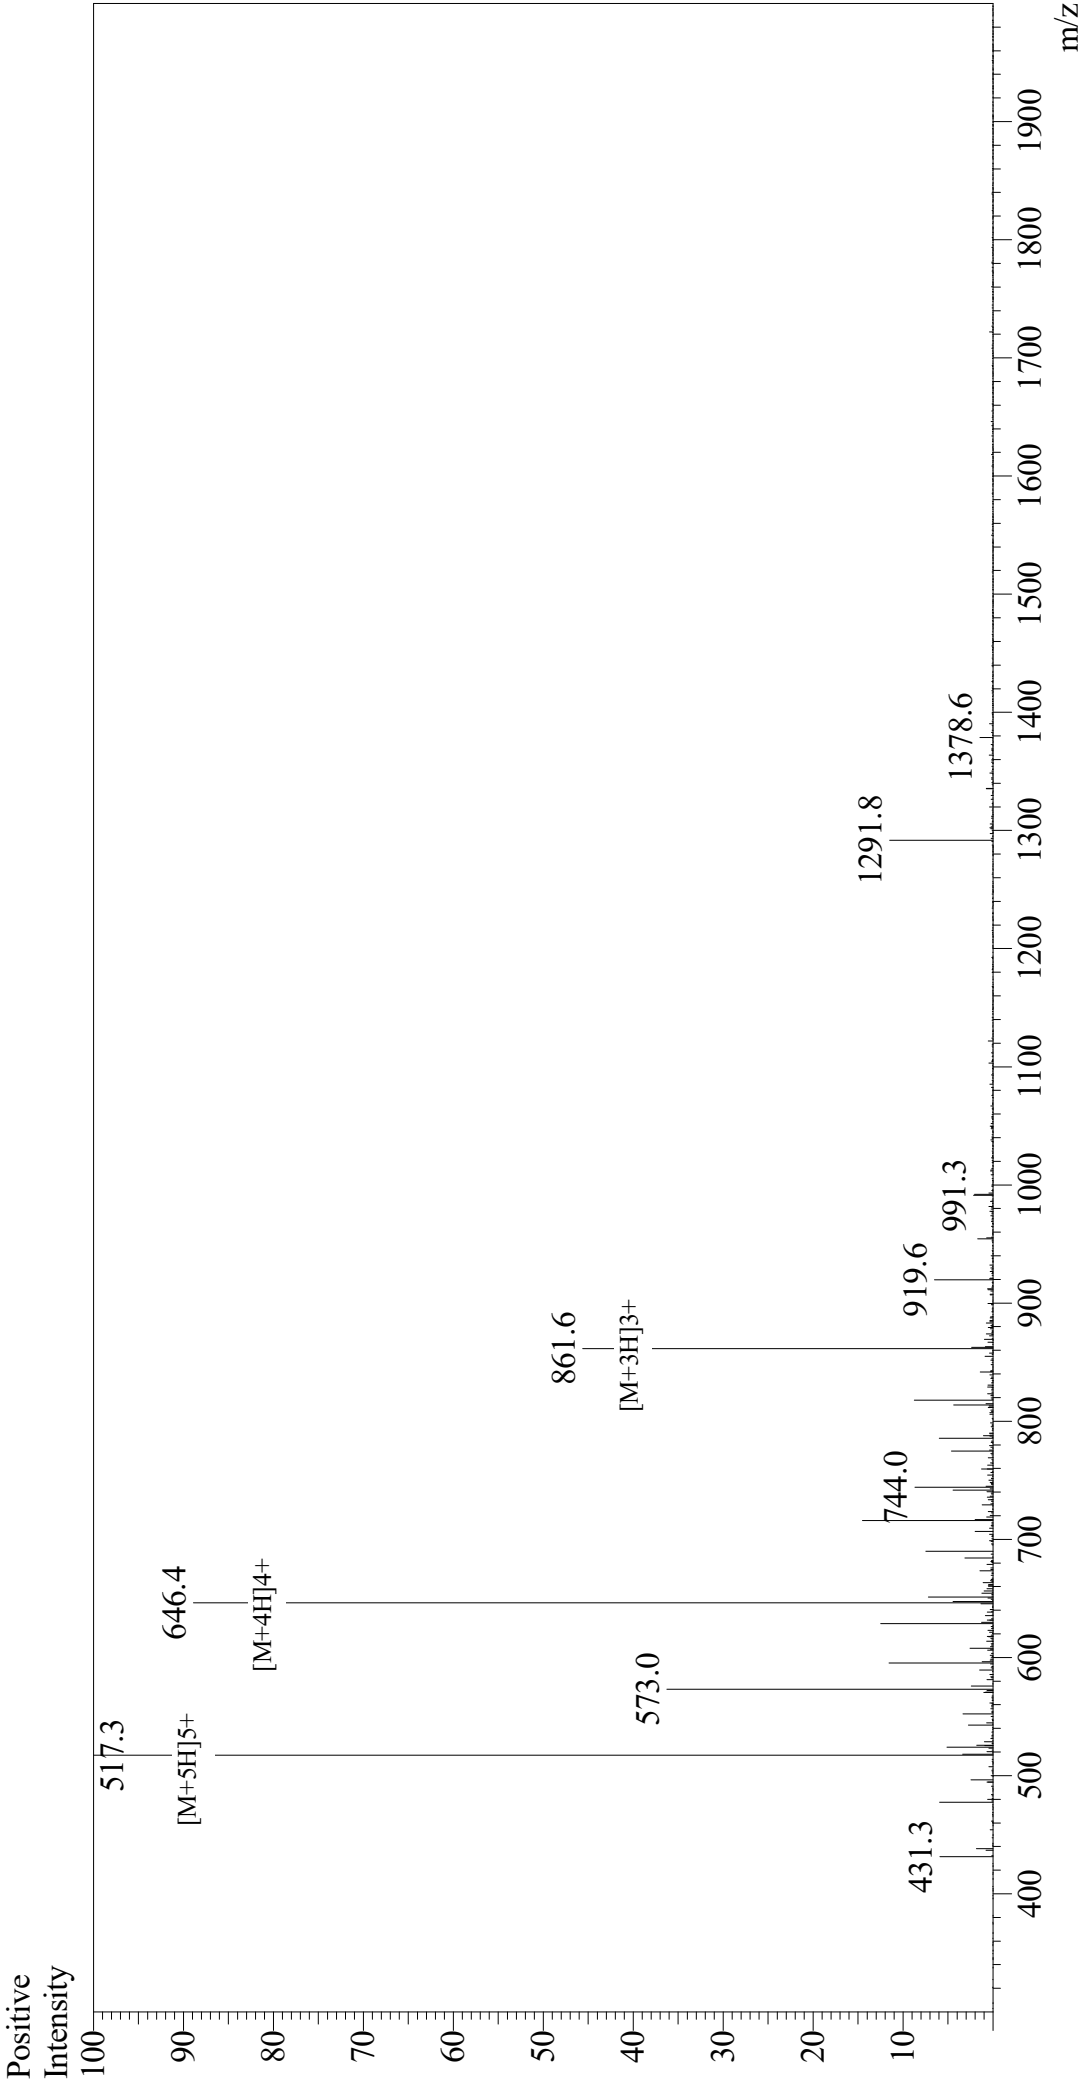

Sample Information

Acquired by : Gary
 Month-Day Processed : 09/01/19
 Time Processed : 03:05:16 PM
 Injection Volume : 0.3
 Sample Name : MOG(35-55)
 Cat. No. : RP10245
 Lot. No. : E7291319H
 Theoretical MW : 2581.98
 Observed MW : 2581.5

Interface : ESI
 Nebulizing Gas Flow : 1.5L/min
 CDL Temp : 250
 Block Temp : 200

Equipment : GK11010007
 Interface Bias : +4.5 kV
 Drying Gas Flow : 5 L/min
 T.Flow : 0.2 ml/min
 B.conc : 50%H2O/50%MeOH