

Sample Name :Amylin, human, amide
 Cat No.: RP11278
 Lot No.:E6380720B
 Time Processed :15:55:18
 Month-Day-Year Processed :02/22/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
50.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

mV

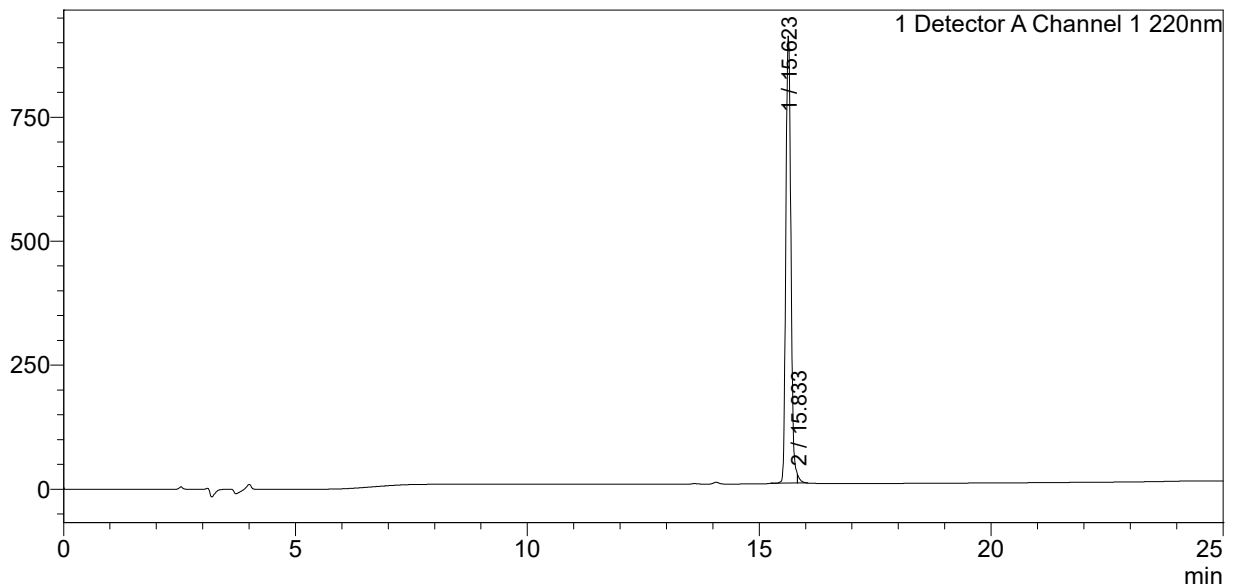

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.623	6866790	901480	99.201
2	15.833	55307	15783	0.799
Total		6922097	917263	100.000