

Sample Name :Melittin

Cat. No. : RP10290 Lot. No. : PE5351805

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

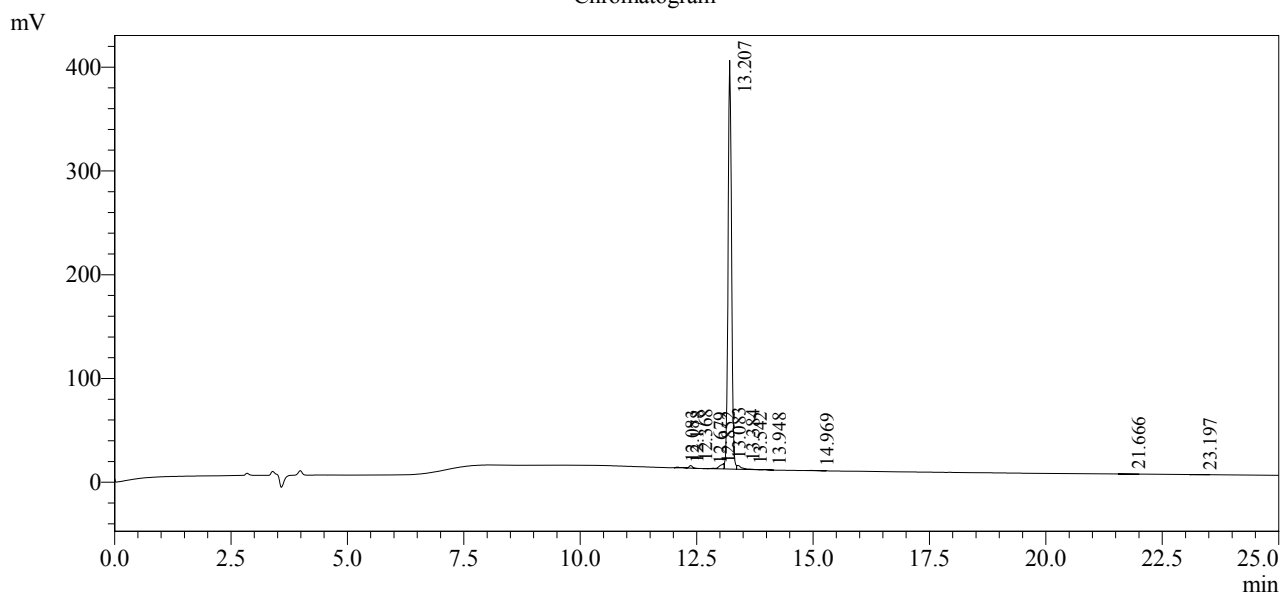

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.083	3205	655	0.150
2	12.178	1399	375	0.065
3	12.368	12156	2436	0.568
4	12.679	240	59	0.011
5	12.852	3147	547	0.147
6	13.083	32525	5049	1.521
7	13.207	2047955	393842	95.744
8	13.384	23062	3629	1.078
9	13.542	4978	649	0.233
10	13.948	2087	381	0.098
11	14.969	2777	246	0.130
12	21.666	3742	365	0.175
13	23.197	1722	94	0.081
Total		2138994	408326	100.000