

Sample Name :SV40 large T antigen NLS  
 Cat. No. : RP20414  
 Lot. No. : PE3741803

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

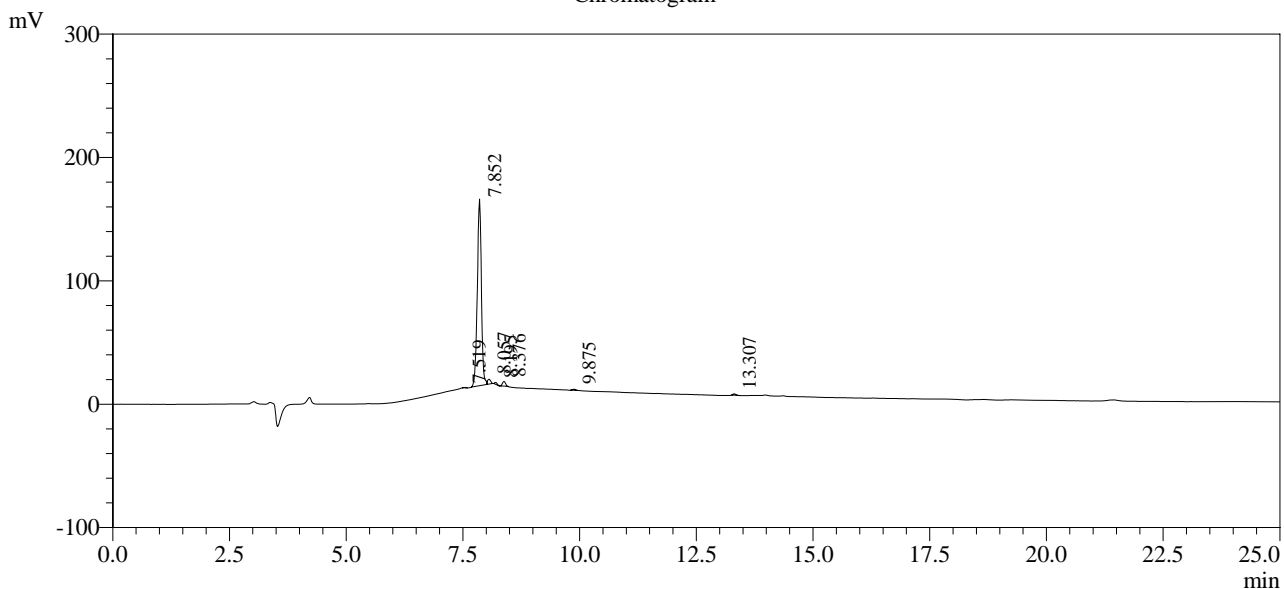

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	7.519	948	276	0.097
2	7.852	924209	151263	95.002
3	8.057	17395	3882	1.788
4	8.195	5390	1428	0.554
5	8.376	17085	3741	1.756
6	9.875	3367	766	0.346
7	13.307	4434	1011	0.456
Total		972827	162367	100.000