

Sample Name : 43Gap 26, Connexin Mimetic
 Cat. No. : RP20274
 Lot. No. : E2094220F
 Time Processed : 8:18:11
 Month-Day-Year Processed : 06/30/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010011

Chromatogram

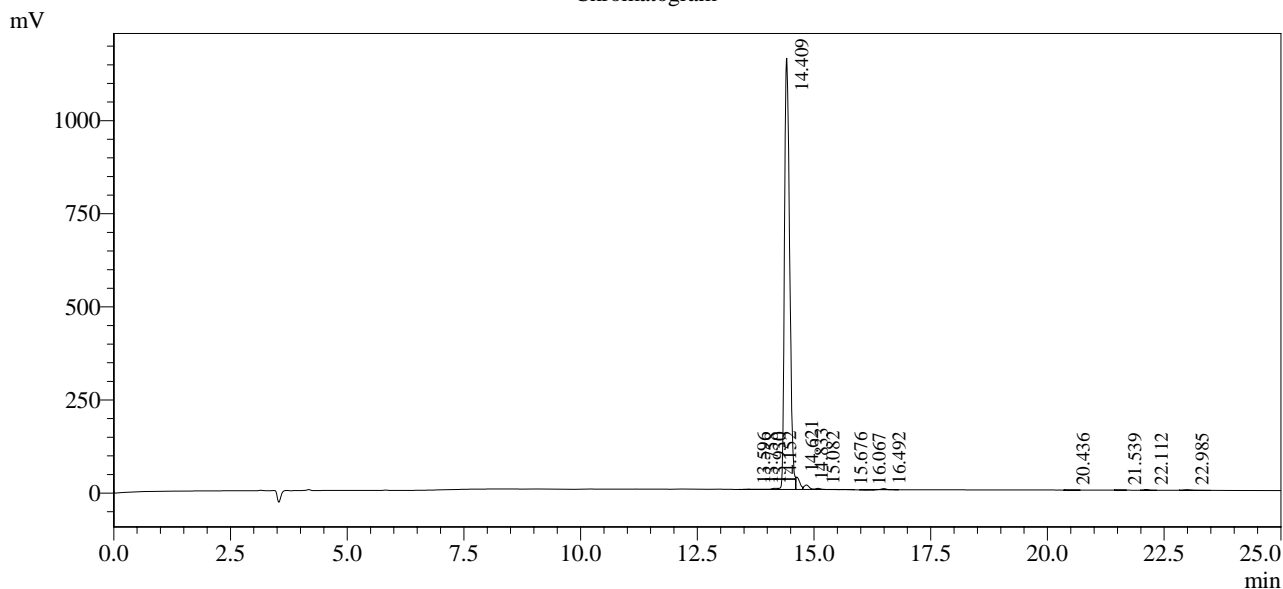

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.596	5028	643	0.054
2	13.758	3009	386	0.032
3	13.930	4535	521	0.048
4	14.152	26196	3149	0.280
5	14.409	8959121	1157816	95.705
6	14.621	187078	33291	1.998
7	14.833	94442	12208	1.009
8	15.082	29634	3240	0.317
9	15.676	1908	229	0.020
10	16.067	1521	183	0.016
11	16.492	21622	2935	0.231
12	20.436	1071	106	0.011
13	21.539	1603	234	0.017
14	22.112	9476	1464	0.101
15	22.985	14944	1281	0.160
Total		9361187	1217686	100.000