

Sample Name : Bradykinin  
 Cat.No : RP11129  
 Lot.No : E8619920L  
 Time Processed: 15:32:31  
 Year-Month-Day: 2020/12/6

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min

<<Detector A>>  
 Wavelength Ch1 : 220 nm

<<LC Time Program>>


Time	Module	Command	Value	Comment
0.01	Pumps	Solvent B Conc.	5	
25.00	Pumps	Solvent B Conc.	65	
25.01	Pumps	Solvent B Conc.	95	
27.00	Pumps	Solvent B Conc.	95	
27.01	Pumps	Solvent B Conc.	5	
33.00	Pumps	Solvent B Conc.	5	
33.01	Controller	Stop		

<<Column Performance>>

<Detector A>  
 Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010015

<Chromatogram>

mV

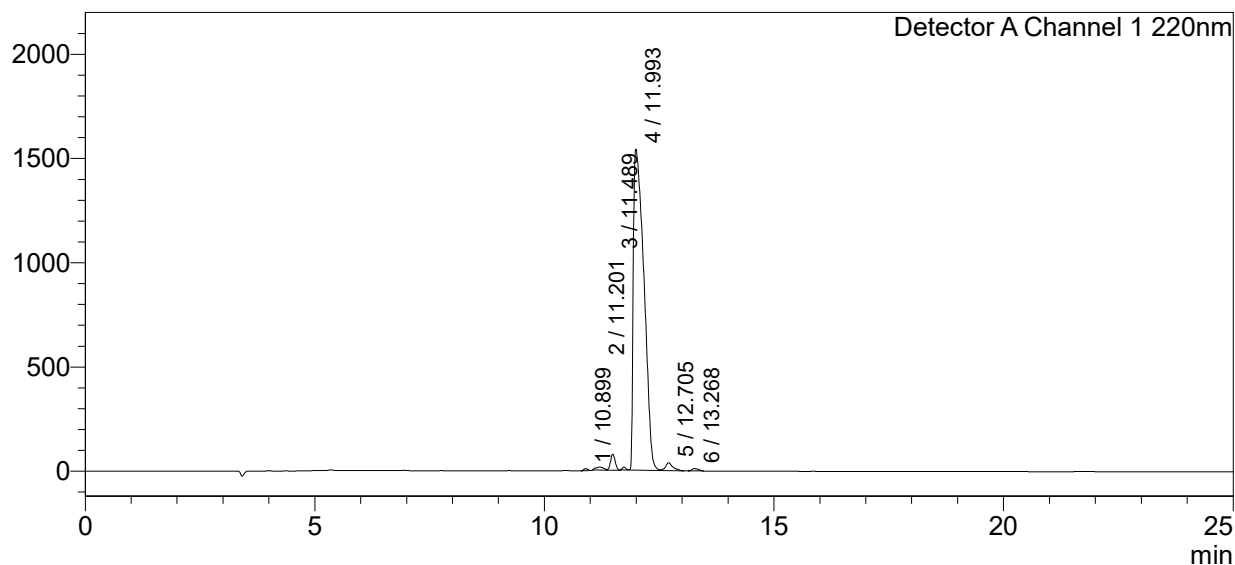

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.899	57117	9341	0.220
2	11.201	174427	15057	0.671
3	11.489	529268	76402	2.036
4	11.993	24695821	1539477	95.023
5	12.705	425678	38094	1.638
6	13.268	107045	11568	0.412
Total		25989357	1689938	100.000